

# **Illuminance Spectrophotometer**

## **CL-500A**

### **Instruction Manual**



Please read before  
using the instrument.



**KONICA MINOLTA**

# Safety Symbols

---

The following symbols are used in this manual to prevent accidents which may occur as result of incorrect use of the instrument.



Denotes a sentence regarding a safety warning or note.  
Read the sentence carefully to ensure safe and correct use.



Denotes a prohibited operation.  
The operation must never be performed.



Denotes an instruction.  
The instruction must be strictly adhered to.



Denotes a prohibited operation.  
Never disassemble the instrument.



Denotes an instruction.  
Always disconnect the AC adapter from the AC outlet.



This symbol indicates A.C.



This symbol indicates D.C.

## Notes on this Manual

- Copying or reproduction of all or part of the contents of this manual without KONICA MINOLTA SENSING's permission is strictly prohibited.
- The contents of this manual are subject to change without prior notice.
- Every effort has been made in the preparation of this manual to ensure the accuracy of its contents. However, should you have any questions or find any errors, please contact a KONICA MINOLTA SENSING-authorized service facility.
- KONICA MINOLTA SENSING will not accept any responsibility for consequences arising from the use of the instrument.

# Safety Precautions

To ensure correct use of this instrument, read the following points carefully and adhere to them.

After you have read this manual, keep it in a safe place where it can be referred to anytime a question arises.

|  <b>WARNING</b>                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                     |  | (Failure to adhere to the following points may result in death or serious injury.)                                                                                                                                                                                                                                                                                                                                             |  |
|--------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|--|--------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|--|
|  Do not use the instrument in places where flammable or combustible gases (gasoline etc.) are present. Doing so may cause a fire.                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                   |  |  Always use the AC adapter supplied as a standard accessory or the optional AC adapter, and connect it to an AC outlet of the rated voltage and frequency. If an AC adapter other than those specified by KONICA MINOLTA SENSING is used, it may result in damage to the unit, fire or electric shock.                                        |  |
|                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                      |  |                                                                                                                                                                                                                                                                                                                                                                                                                                |  |
|  In the event that the battery leaks, take the following actions. <ul style="list-style-type: none"> <li>• Immediately move the instrument away from any open flames. There is a risk of fire or explosion from the leaked fluid or gas igniting.</li> <li>• If the leaked fluid gets in the eyes, immediately and thoroughly wash the eyes with clean water, such as tap water, without rubbing them and then seek medical attention.</li> <li>• Do not taste the leaked fluid or put it in your mouth. In such a case, immediately wash the mouth with tap water and consult a physician.</li> <li>• If the leaked fluid is on the body or clothes, thoroughly wash it off with water.</li> </ul> |  |  If the instrument will not be used for a long time, disconnect the AC adapter from the AC outlet. Accumulated dirt or water on the prongs of the AC adapter's plug may cause a fire and should be removed.                                                                                                                                   |  |
|                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                      |  |  Do not disassemble or modify the instrument or the AC adapter. Doing so may cause a fire or electric shock.                                                                                                                                                                                                                                  |  |
|                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                      |  |  Take special care not to allow liquid or metal objects to enter the instrument. Doing so may cause a fire or electric shock. Should liquid or metal objects enter the instrument, turn the power OFF immediately, disconnect the AC adapter from the AC outlet, and contact the nearest KONICA MINOLTA SENSING-authorized service facility. |  |
|  The instrument should not be operated if it is damaged or the AC adapter is damaged, or if smoke or odd smells occur. Doing so may cause a fire. In such situations, turn the power OFF immediately, disconnect the AC adapter from the AC outlet and contact the nearest KONICA MINOLTA SENSING-authorized service facility.                                                                                                                                                                                                                                                                                                                                                                    |  |  Do not insert or disconnect the AC adapter with wet hands. Doing so may cause electric shock.                                                                                                                                                                                                                                              |  |



## CAUTION

(Failure to adhere to the following points may result in injury or damage to the instrument or other property.)



Setup the environment so there is an outlet near the instrument and the power plug can be easily plugged in and unplugged.



When cleaning the instrument, unplug the power plug from the outlet. Not doing so may cause electric shock.

# Introduction

Thank you for purchasing this KONICA MINOLTA SENSING instrument.

This instrument is a compact, lightweight, portable illuminance spectrophotometer ideal for evaluating CRI (color rendering index).

## **Packing materials of the product**

Be sure to keep all packing materials used for shipping the product (cardboard box, cushioning material, plastic bags, etc.).

This instrument is a precision measuring instrument. When transporting the instrument to a service facility for maintenance or for other reasons, be sure to use the packing materials to minimize shock or vibration.

If the packing materials are lost or damaged, contact a KONICA MINOLTA SENSING-authorized service facility.

## Notes on Use

---

Always use the instrument correctly. If the instrument is used in a manner not described in this instruction manual, it may cause injury, electrocution, or damage to the instrument itself.

## Operating Environment

Use the instrument at an ambient temperature between -10°C and 40°C and a relative humidity of 85% or less (at 35°C) with no condensation.

Be sure to use the instrument within these ranges. Do not use it in areas of rapid temperature changes.

- Do not leave the instrument in direct sunlight or near heat sources such as stoves, etc. The internal temperature of the instrument may become much higher than the ambient temperature in such cases.
- Do not use the instrument in areas where dust, cigarette smoke, or chemical gases are present. Doing so may cause deterioration in performance or a breakdown.
- Do not use the instrument near equipment which produces a strong magnetic field (such as speakers etc.).
- The instrument belongs to pollution level 2 products (equipment which may cause temporary electrical hazards due to contamination or condensation or products which are used in such an environment).
- Do not use the instrument at altitudes higher than 2,000 m.
- The AC adapter supplied as a standard accessory have been designed exclusively for indoor use. They should never be used outdoors because rain or other factors may damage the instrument.

## Measurement

- When not using the instrument for a long period of time, blow off dirt or dust on the Receptor Window with a blower before use.
- The spherical summit of the receptor window is used as the illuminance reference plane.
- When using the instrument for long periods of time, the measurement value may change depending on changes in the environment. Therefore, in order to achieve accurate measurements, we recommend that zero calibration be done regularly using the Cap.

## Power Source

- When the instrument is not being used, turn the power switch OFF.
- Charge the instrument using the AC adapter or from a PC via the USB cable.
- Always use the AC adapter supplied as a standard accessory and connect it to an AC outlet of the rated voltage and frequency. Use an AC power supply of the rated supply voltage (within  $\pm 10\%$ ).

---

## System

- Do not subject the instrument to strong impacts or vibrations. Doing so may cause deterioration in performance or a breakdown.
- Since the receptor window is an extremely precise optical component, great care should be taken to prevent it from getting dirty or exposing it to impacts. Be sure to attach the cap when the instrument is not in use.
- The instrument may cause interference if used near a television, radio, etc.
- When the instrument is exposed to strong external static electricity, the LCD may go blank or the measurement result may not be displayed properly. If the instrument is communicating with an external device, the communication may be interrupted. In these cases, turn the power OFF and then turn it ON again. If black smudges appear on the LCD, wait until they disappear naturally.
- When turning the power OFF and then ON again, wait several seconds after turning the power OFF.

## Internal Lithium-Ion Battery

- The operating time per charge with the internal lithium-ion battery is 6 hours. (When new, fully charged)
- When purchased, the battery is not charged. Refer to page E-14 “Connecting the AC Adapter” and charge it correctly.
- Charge the battery at a temperature from 5°C to 35°C.
- The internal lithium-ion battery is fully charged in about 3.6 hours. There is no worry about overcharging the battery.

**Notes** • Do not try to replace the internal lithium-ion battery yourself. Contact a KONICA MINOLTA SENSING-authorized service facility.

## Notes on Storage

---

- The instrument should be stored at a temperature between -10°C and 45°C and a relative humidity of 85% or less (at 35°C) with no condensation. Do not store the instrument in areas subject to high temperatures, high humidity, sudden changes in temperature, or where condensation may occur, because these circumstances may cause a breakdown. We recommend you store the instrument with a drying agent at a temperature around 20°C.
- Do not leave the instrument inside a car such as in the cabinet or trunk. Otherwise, the temperature and/or humidity may exceed the allowable range for storage during midsummer or midwinter, resulting in a breakdown.
- Keep the packing materials used for shipment and use them to transport the instrument. This protects the instrument from sudden changes in temperature and from vibration and shock.
- Do not store the instrument in areas where dust, cigarette smoke, or chemical gases are present. Doing so may cause deterioration in performance or a breakdown.
- Be sure to keep all packing materials (cardboard box, cushioning material, plastic bags, etc.). They can be used to protect the instrument during transportation to the service facility for maintenance (re-calibration etc.).
- When not using the instrument for a long period of time, we recommend you give the instrument an auxiliary charge every year to protect the battery from overdischarge.

## Notes on Cleaning

---

- When the instrument is dirty, wipe it with a soft, clean dry cloth. Never use solvents such as thinner or benzene.
- If there is dust or dirt on it, use a blower to blow it off or gently wipe it with a soft, clean dry cloth. Never use solvents such as thinner or benzene. If you are unable to remove dirt from the instrument or should the instrument become scratched, contact a KONICA MINOLTA SENSING-authorized service facility.
- Should the instrument break down, do not try to disassemble and repair it by yourself. Contact a KONICA MINOLTA SENSING-authorized service facility.

## Disposal Method

---

- Make sure that the instrument, its accessories, and the packing materials are either disposed of or recycled correctly in accordance with local laws and regulations.

# Table of Contents

|                             |                                                                                                                                                                          |
|-----------------------------|--------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| Before Using the Instrument | <b>Safety Precautions..... E-1</b>                                                                                                                                       |
| Preparation for Measurement | <b>Introduction ..... E-3</b>                                                                                                                                            |
|                             | Notes on Use ..... E-3                                                                                                                                                   |
|                             | Notes on Storage ..... E-5                                                                                                                                               |
|                             | Notes on Cleaning ..... E-5                                                                                                                                              |
|                             | Disposal Method ..... E-5                                                                                                                                                |
| Measurement                 | <b>Chapter 1 - Before Using the Instrument ..... E-7</b>                                                                                                                 |
|                             | Standard Accessories ..... E-8                                                                                                                                           |
|                             | Optional Accessories ..... E-8                                                                                                                                           |
|                             | System Diagram ..... E-9                                                                                                                                                 |
|                             | Names and Functions of Parts ..... E-10                                                                                                                                  |
|                             | Attaching the Wrist strap and the Cap ..... E-13                                                                                                                         |
|                             | Connecting the AC Adapter ..... E-14                                                                                                                                     |
|                             | Turning Power ON/OFF ..... E-16                                                                                                                                          |
| Other Functions             | <b>Chapter 2 - Preparation for Measurement ..... E-19</b>                                                                                                                |
|                             | Flow of Measurement ..... E-20                                                                                                                                           |
|                             | Zero Calibration ..... E-21                                                                                                                                              |
|                             | Setting the Measurement Conditions <span>Display Type</span> <span>Color Space</span> <span>Meas. Time</span> <span>Observer</span> <span>Illum. Units</span> ..... E-22 |
|                             | User calibration ..... E-29                                                                                                                                              |
| Troubleshooting             | <b>Chapter 3 - Measurement..... E-31</b>                                                                                                                                 |
|                             | Measurement ..... E-32                                                                                                                                                   |
|                             | About Targets ..... E-34                                                                                                                                                 |
|                             | Measured Data Operations ..... E-39                                                                                                                                      |
| Appendix                    | <b>Chapter 4 - Other Functions ..... E-43</b>                                                                                                                            |
|                             | Connecting to a PC ..... E-44                                                                                                                                            |
|                             | CL-500A Settings ..... E-46                                                                                                                                              |
|                             | Checking CL-500A Information ..... E-57                                                                                                                                  |
|                             | <b>Chapter 5 - Troubleshooting ..... E-61</b>                                                                                                                            |
|                             | Error Messages ..... E-62                                                                                                                                                |
|                             | Checking for Malfunction ..... E-64                                                                                                                                      |
|                             | Special Startup Procedures ..... E-65                                                                                                                                    |
|                             | <b>Chapter 6 - Appendix ..... E-67</b>                                                                                                                                   |
|                             | Luminance Measurement Capabilities..... E-68                                                                                                                             |
|                             | LvTΔuv ..... E-69                                                                                                                                                        |
|                             | Dominant wavelength/Excitation purity ..... E-70                                                                                                                         |
|                             | External Dimensions ..... E-71                                                                                                                                           |
|                             | Specifications ..... E-72                                                                                                                                                |






# Before Using the Instrument

|                                                         |      |
|---------------------------------------------------------|------|
| Standard Accessories .....                              | E-8  |
| Optional Accessories .....                              | E-8  |
| System Diagram .....                                    | E-9  |
| Names and Functions of Parts .....                      | E-10 |
| Control Panel/Screen Display (LCD Screen).....          | E-12 |
| Attaching the Wrist strap and the Cap .....             | E-13 |
| Attaching the Wrist strap and the Cap .....             | E-13 |
| Attaching the Cap (Without the Strap).....              | E-13 |
| Connecting the AC Adapter .....                         | E-14 |
| Attaching the AC Adapter .....                          | E-14 |
| Battery Warning .....                                   | E-15 |
| When the Low Battery Voltage Message is Displayed ..... | E-15 |
| Turning Power ON/OFF .....                              | E-16 |
| Auto Power Off Feature .....                            | E-16 |
| When First Turning ON the CL-500A .....                 | E-17 |

# 1

## Standard Accessories


| Name                                                                                                     |                                                                                     | Description                                                                                                                                                                                                                                                                                                                                       |
|----------------------------------------------------------------------------------------------------------|-------------------------------------------------------------------------------------|---------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| Cap (with Strap)<br>T-A13                                                                                |    | Attaches to the receptor window when performing zero calibration. Also attached to protect the receptor window during storage.                                                                                                                                                                                                                    |
| Wrist Strap<br>CR-A73                                                                                    |    | Prevents accidental dropping of the instrument.                                                                                                                                                                                                                                                                                                   |
| AC Adapter*<br>AC-A305F (North and South America and Taiwan)<br>FW7711/0.7 (Europe)<br>MM611 (Singapore) |    | Used to supply power from an AC outlet to the instrument.<br>(North and South America and Taiwan)<br>Input: 100-240 V $\sim$ 50-60 Hz 0.2 A<br>Output: 5 V $\equiv$ 1 A<br>(Europe)<br>Input: 100-240 V $\sim$ 50-60 Hz 100 mA<br>Output: 5 V $\equiv$ 700 mA<br>(Singapore)<br>Input: 100-240 V $\sim$ 50-60 Hz<br>Output: 5.2 V $\equiv$ 500 mA |
| USB Cable<br>IF-A17                                                                                      |    | Used to connect the instrument to a personal computer (PC).<br>When using AC Adapter, power can be supplied through the cable.                                                                                                                                                                                                                    |
| Soft Case<br>FD-A05                                                                                      |  | Used to store the instrument together with accessories.                                                                                                                                                                                                                                                                                           |
| Data Management Software<br>CL-S10w                                                                      |  | Software that can operate the instrument from a PC, perform measurements and data processing, and file management.                                                                                                                                                                                                                                |

\* Form differs according to region.

## Optional Accessories

| Name           | Description                                    |
|----------------|------------------------------------------------|
| Hood<br>CL-A11 | Used to suppress the effects of outdoor light. |


# System Diagram

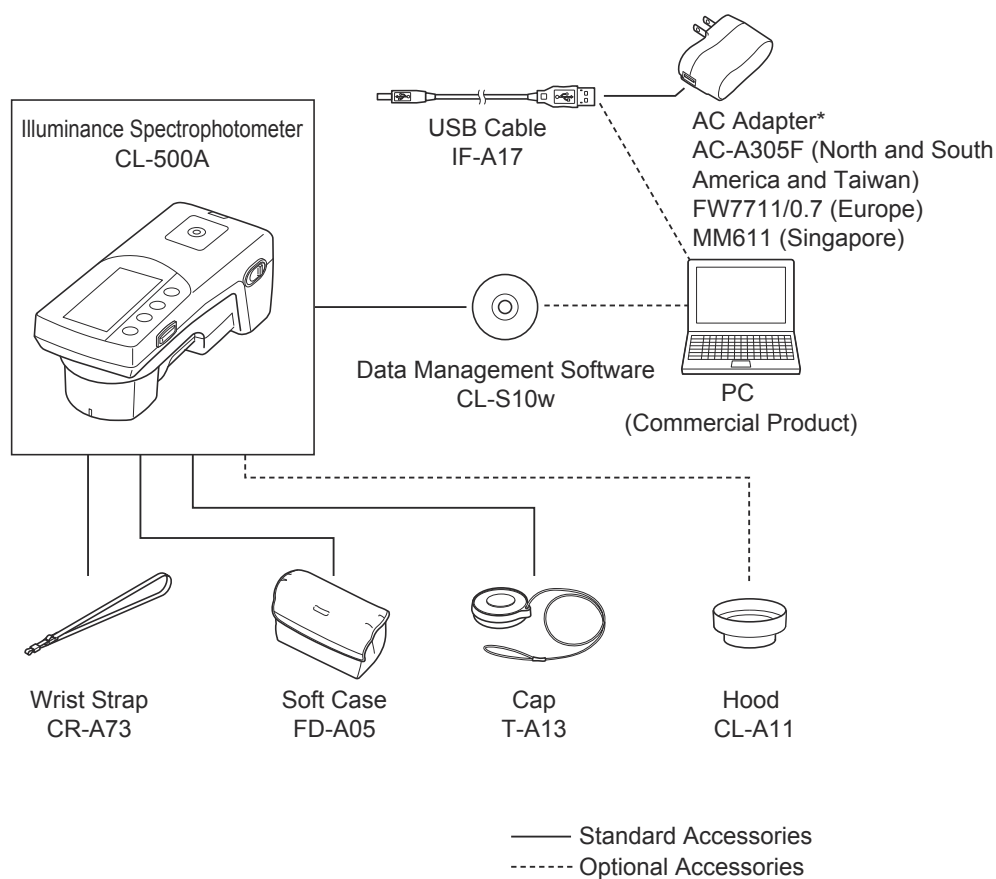

\* Form differs according to region.

# Names and Functions of Parts


| Name                       | Function                                                                                                                                                                                               | Reference Page  |
|----------------------------|--------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|-----------------|
| 1. LCD screen              | Displays setting items, measurement results, and messages.<br>For details, refer to “Control Panel”.                                                                                                   | Page E-12       |
| 2. Control panel           | Used to switch screens or select/determine/save setting items.                                                                                                                                         | Page E-12       |
| 3. Measuring button        | Press this button to perform calibration or measurement.                                                                                                                                               | Page E-21, E-32 |
| 4. Receptor window         | Receptor for illuminance measurement.                                                                                                                                                                  |                 |
| 5. USB connection terminal | Used to connect the instrument to a PC with the optional USB cable.                                                                                                                                    | Page E-44       |
|                            | When using AC Adapter, power can be supplied through the USB cable.                                                                                                                                    | Page E-14       |
| 6,7. Tripod socket         | Used to set this instrument on tripod or jig.                                                                                                                                                          |                 |
| 8. Power switch            | Used to turn ON/OFF power. Setting this switch to “○” turns the power OFF, and setting it to “  ” turns the power ON. | Page E-16       |
| 9. Strap hook              | For attachment of the wrist strap (CR-A73).                                                                                                                                                            | Page E-13       |

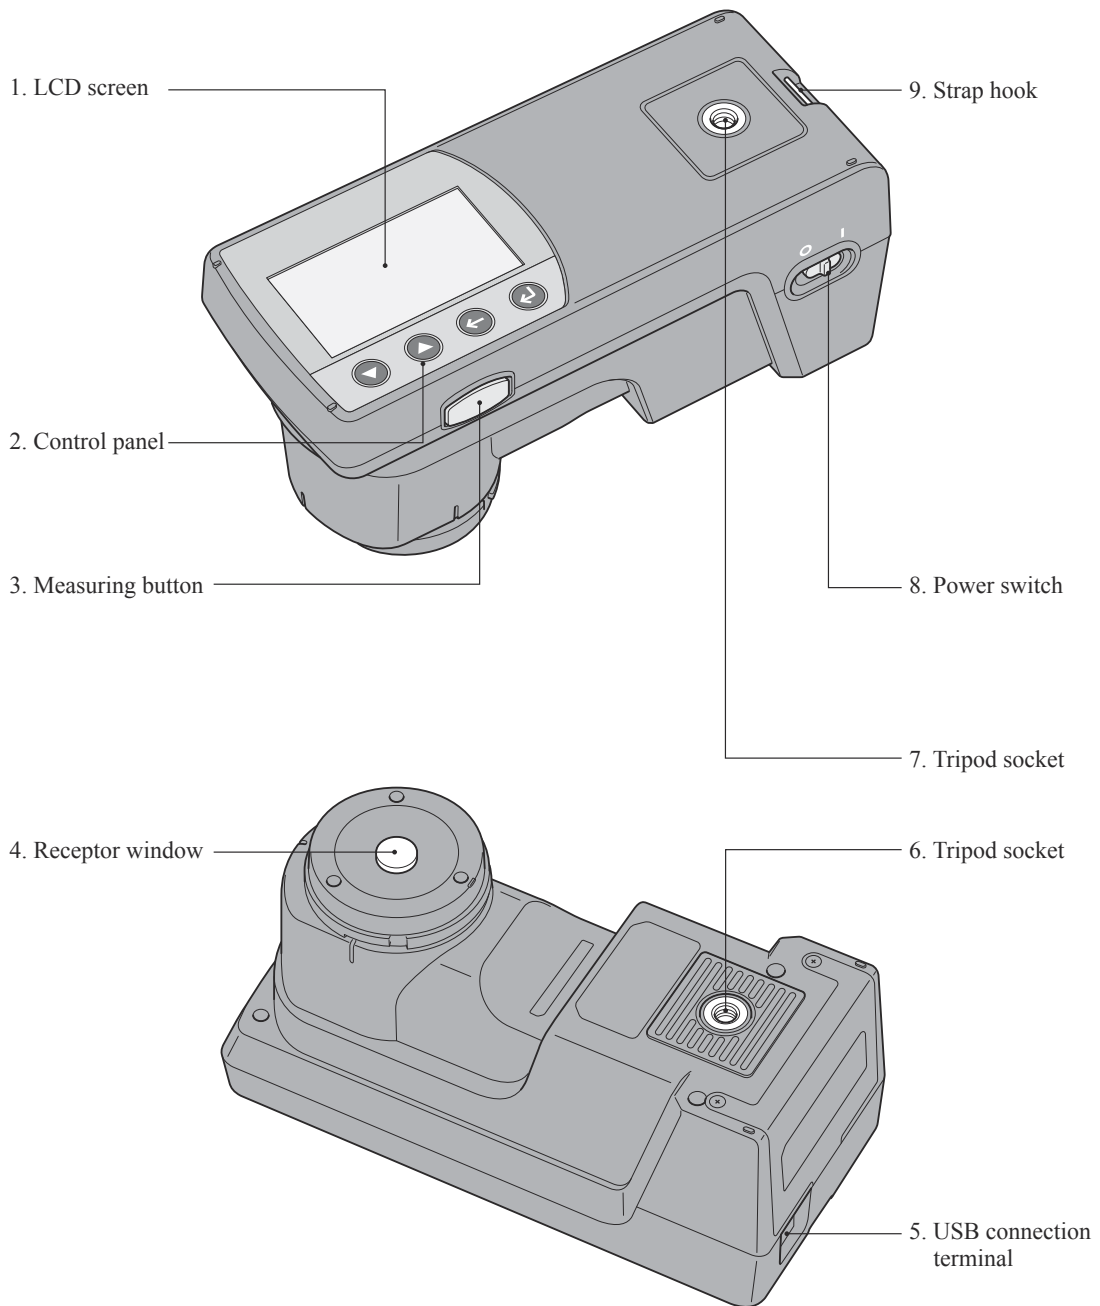

# Control Panel/Screen Display (LCD Screen)

## Control Panel


Located on the upper surface of the instrument is the LCD screen for displaying measurement results with the instrument and messages, and the control buttons for configuring the various settings for measurements and switching the display.

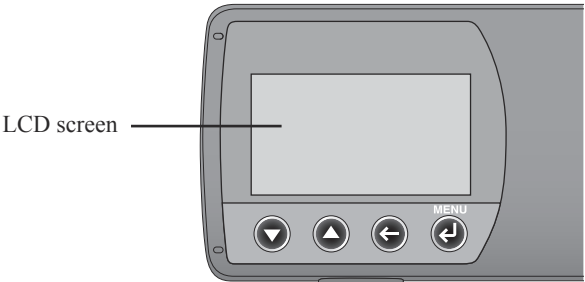


## Screen Display (LCD Screen)

The LCD screen displays setting items, measurement results, and messages. The basic screen configuration is shown in the figures below.

(Measurement Screen)

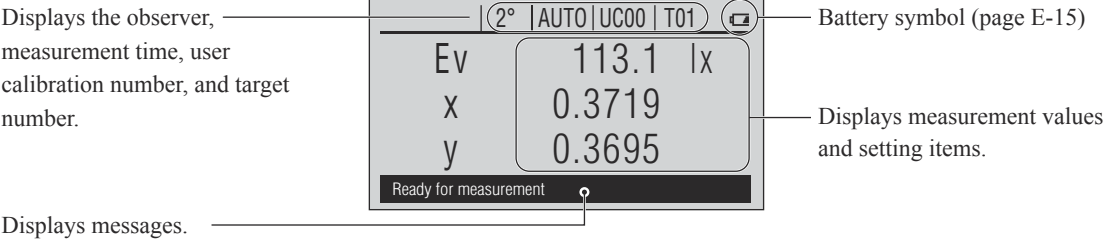

(Configuration Screen)

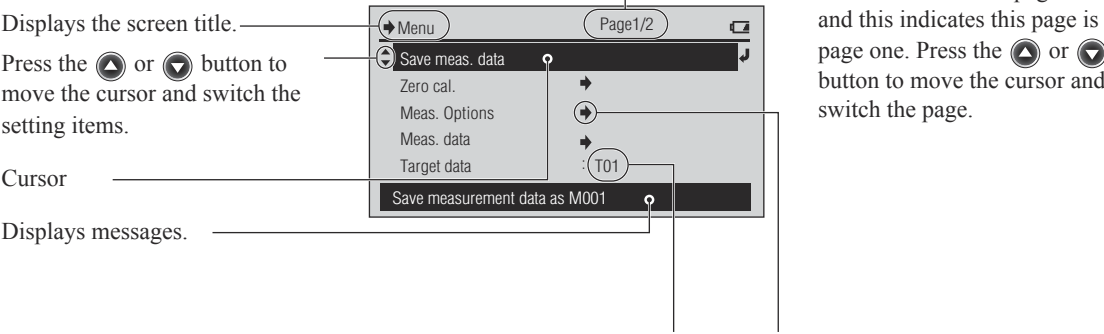

For the left item (“Target data” here), indicates settings on the next screen. Press the (Enter)/MENU button to go to the next screen.


For the left item (“Meas. Options” here), indicates settings on the next screen. Press the (Enter)/MENU button to go to the next screen.

# Attaching the Wrist strap and the Cap

## Attaching the Wrist strap and the Cap

If you are using the wrist strap, attach the cap to the strap as shown below.


- 1 Pass the wrist strap through loop of the cap string and then through the strap hook, and then pass one end of the wrist strap through the other.

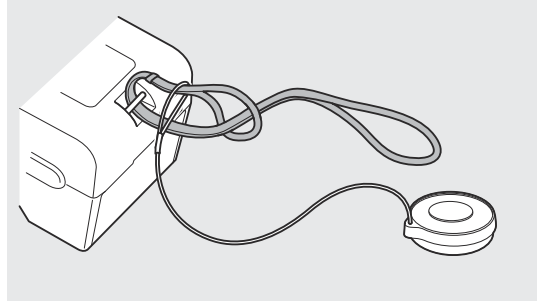


## Attaching the Cap (Without the Strap)

If you are using the wrist strap, attach the cap to the main body as follows.


- 1 Untie the knot holding the cap string to the cap, and remove the string from the cap.

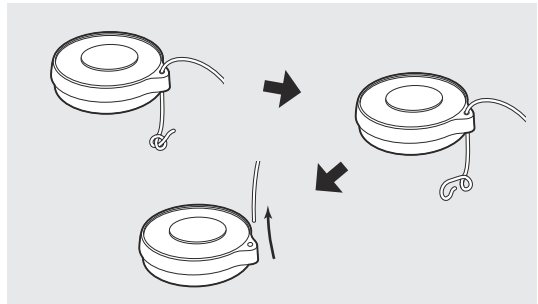

- 2 Attach the string to the strap hook as shown in the illustration.

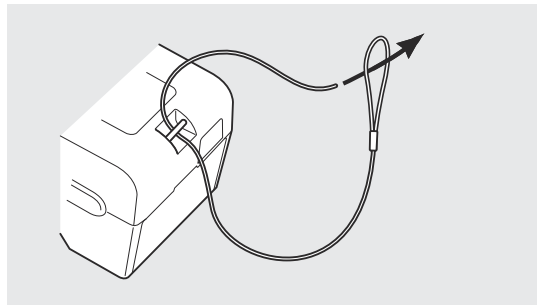

- 3 Pass the string back through the hole in the cap, and tie a knot at the end of the string so that the cap cannot come off.

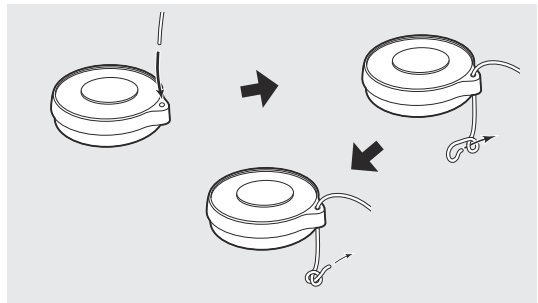

## Connecting the AC Adapter

This instrument runs on its internal lithium-ion battery, but we recommended using the AC adapter or USB bus power when using the instrument for a long period of time.

The internal lithium-ion battery is charged by the AC adapter or USB bus power.


- Notes**
- Always use the included AC adapter as the instrument's AC adapter.
- Memo**
- The AC adapter connects via the USB cable (IF-A17).
  - USB bus power is a way to supply power from a PC through the USB cable.

## Attaching the AC Adapter


### [Operating Procedure]

The AC adapter can be plugged in or unplugged even when the instrument's power is ON, but here it is connected with the power turned OFF.


- 1 Make sure that the power is OFF (Power switch is set to "O").**

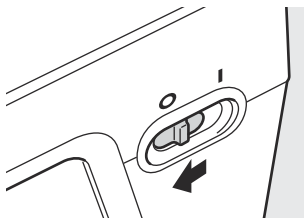


- 2 Plug the USB cable's connector (A type) into the AC adapter.**

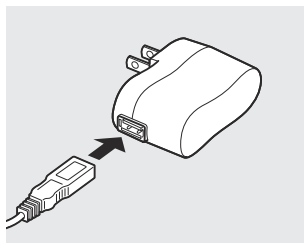

- 3 Connect the USB cable's connector (B type) to the USB connection terminal.**

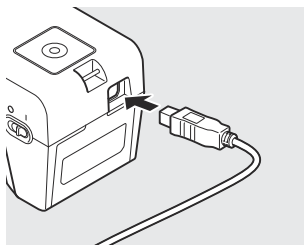


- 4 Insert the AC adapter power plug to an AC outlet (100 to 240 VAC, 50-60 Hz).**

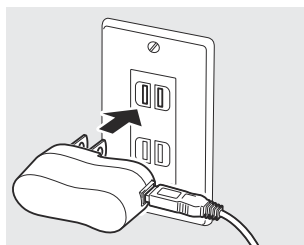



## Battery Warning

When the battery’s capacity runs out when running on the internal lithium-ion battery, the battery symbol on the LCD screen changes to the low battery symbol.

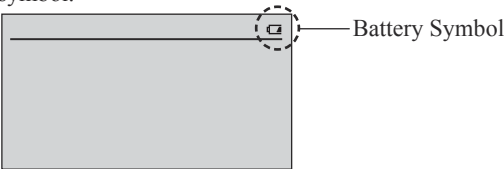

| Battery Symbol                                                                      | State        | Description                                                                                                                                                                                                                                                                                          | Comment                                                                                |
|-------------------------------------------------------------------------------------|--------------|------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|----------------------------------------------------------------------------------------|
|    | Charging     | When charging via the AC adapter or USB bus power, the battery charging symbol is displayed as the battery symbol.<br><b>Memo</b> It is not displayed when the power switch is turned OFF, but the internal lithium-ion battery is still charging. There is no worry about overcharging the battery. | With the power switch turned OFF, the battery can be fully charged in about 3.6 hours. |
|    | Low battery  | Even when this symbol is displayed, you can still continue measurements for a while, but we recommend you soon charge the internal lithium-ion battery via the AC adapter or USB bus power.                                                                                                          | You can measure about 2 hours after this symbol is displayed.                          |
|  | Dead battery | The battery is dead. Use the AC adapter or USB bus power to charge the internal lithium-ion battery.                                                                                                                                                                                                 | You can measure about 15 minutes after this symbol is displayed.                       |
| (No indicator displayed)                                                            | Full battery | The internal lithium-ion battery has sufficient power during battery operation.                                                                                                                                                                                                                      | You can measure about 6 hours with a new, fully charged battery.                       |

## When the Low Battery Voltage Message is Displayed

If you continue using the instrument with the low battery symbol displayed, the low battery voltage message is displayed and the instrument automatically turns off after a few seconds.


Please use the AC adapter or USB bus power immediately. This will charge the internal lithium-ion battery. When battery voltage is low, the instrument may not start up immediately after the AC adapter is connected. In this case, allow the battery to charge for a few minutes and then turn on the instrument.

# Turning Power ON/OFF

## [Operating Procedure]

### Turning power ON


- 1 Slide the Power switch to the “I” side.

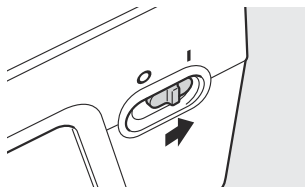

The power is ON.

### Turning power OFF

- 1 Slide the Power switch to the “O” side.

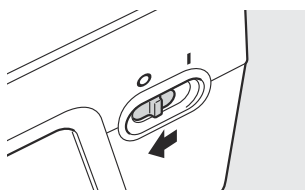

After settings such as the measurement conditions are saved to the instrument, the power turns OFF.

## Auto Power Off Feature

This instrument is equipped with an auto power off feature. When running the instrument on its built-in lithium-ion battery without AC adapter or USB bus power, auto power off automatically turns power OFF if no control button operation is performed for more than 15 minutes.

The settings such as the measurement conditions are saved when the power is turned OFF, so the next time the power is turned ON, you can start operating the instrument with the same settings as when last turned OFF.


- Memo**
- When the power is turned OFF with the auto power off feature, the power switch is left on the “I” side. Slide it to the “O” side.
  - You also can configure the instrument to disable Auto Power Off. (Page E-51)

# When First Turning ON the CL-500A

The first time you turn ON the instrument after purchase, the <Language> and <Date/Time> screens will appear in English.


You can select and change the display language from a total of three languages including English.

(LCD Screen)


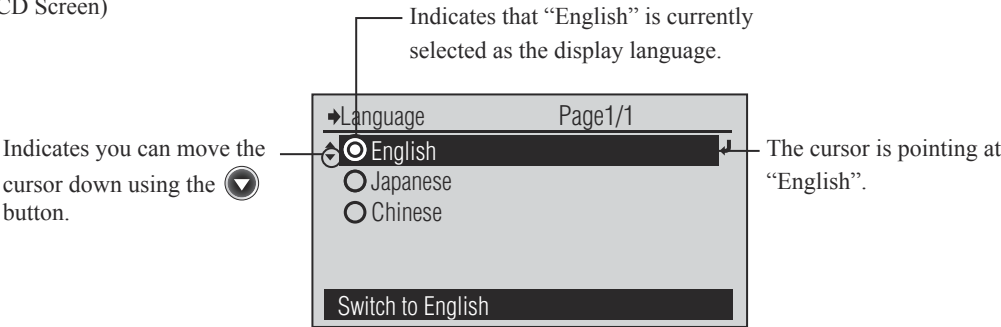


## [Operating Procedure]


- 1 Move the cursor to the language you wish to select with the or button, then press the (Enter)/MENU button.
- 2 Move the cursor to “OK” with the button, then press the (Enter)/MENU button.
- 3 Move the cursor to “Date/Time” with the or button and press the (Enter)/MENU button.
- 4 Set the year/month/day/hour/minute/second. Press the button to increase the selected value or the button to decrease it. Holding down either button will change the selected value at high speed. Press the (Enter)/MENU button for each value to apply its setting.



The <Confirm Change> screen is displayed.




The <Date/Time> configuration screen is displayed.



This applies the changes you made to the setting and moves the cursor to the next value to the right.

### **Memo**

Note that you cannot move the cursor to the left during the setting procedure.



After the initial screen, the calibration prompt screen is displayed. Select “OK” to run calibration or select “Cancel” and you can skip calibration.



# Preparation for Measurement


|                                                                |      |
|----------------------------------------------------------------|------|
| Flow of Measurement.....                                       | E-20 |
| Basic procedure.....                                           | E-20 |
| Optional settings .....                                        | E-20 |
| Zero Calibration.....                                          | E-21 |
| Setting the Measurement Conditions.....                        | E-22 |
| Display Type.....                                              | E-23 |
| Color Space.....                                               | E-24 |
| Custom .....                                                   | E-25 |
| Meas. Time.....                                                | E-26 |
| Observer.....                                                  | E-27 |
| Illum. Units .....                                             | E-28 |
| User calibration.....                                          | E-29 |
| Selecting a User Calibration Channel .....                     | E-29 |
| Changing the Items in the List on the <User cal.> Screen ..... | E-30 |

# Flow of Measurement

## Basic procedure

## Optional settings

Power ON (page E-16)




Zero Calibration (page E-21)

Configure the Display Language and Date/Time (page E-17, E-46)  
\* As necessary, such as when the power is first turned ON

Configure the Measuring Instrument (page E-17, E-46)  
\* As necessary, such as when the power is first turned ON

Configure the Measurement Conditions (page E-22)  
\* As necessary, such as when changing the measurement conditions from the previous time



("Display Type" Options Screen Example)


Select the User Calibration Channel (page E-29)  
\* As required when changing the user calibration channel from what was used previously, etc.

Select the Target (page E-34)  
\* As required during difference measurement when changing the target from what was used previously.

Measurement (page E-32)

Data Saving (page E-32, E-39)

Completion of Measurement (page E-16)



# Zero Calibration


This instrument must perform zero calibration after it is first turned ON or after a fixed amount of time has elapsed from the last zero calibration.

- Memo**
- The reading may fluctuate slightly due to changes in the ambient temperature or due to heat generation caused by the repeated operation of the instrument. In this case, make sure to perform zero calibration regularly.
  - If the ambient temperature changes greatly, the calibration prompt screen may be displayed. In this case, make sure to perform zero calibration.
  - Frequent short zero calibration is recommended for better accuracy when measuring low illuminance.
  - When a fixed amount of time elapses from the last zero calibration, the calibration prompt screen is displayed. This calibration expiry can be changed. You also can disable display of the calibration prompt screen. Refer to page E-52 “Configuring the Zero Calibration Expiry”.


- Notes**
- Allow the instrument to become fully accustomed to the ambient temperature before performing zero calibration.

## [Operating Procedure]

- 1** When the calibration prompt screen is displayed, select “OK”.  
(Move the cursor to “OK” with the  button and press the  (Enter)/MENU button.)




To run calibration when a screen other than the calibration prompt screen is displayed, run it from the <Menu> screen. Refer to page E-22.




The <Zero cal.> screen is displayed.


- 2** Correctly set the cap to the Receptor Window of the instrument.

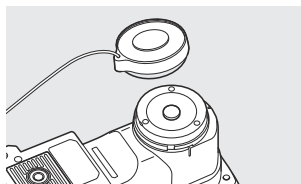


- 3** Push the Measuring button.

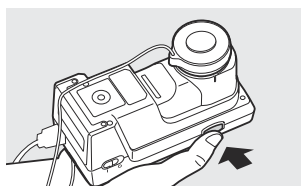

You will hear a beep and see “Calibrating...” displayed.



- 4** You will hear another beep. When “Calibrating...” no longer displays, zero calibration is complete.



A measurement screen is displayed. Or you return to the <Menu> screen.

# Setting the Measurement Conditions

You must configure measurement conditions on the instrument before performing measurements, but each item has been configured with an initial setting, making it possible to measure as-is.

Use the <Meas. Options> screen, which are accessed from the <Menu> screen, to configure measurement option settings.


Move to the <Meas. Options> screen with the procedure below.

As necessary

Change settings.

## [Operating Procedure]

- 1** While the measurement screen is displayed, press the  (Enter)/MENU button.




The <Menu> screen is displayed.

### **Memo**

You can use the <Menu> screen to configure settings for measurement data storage, zero calibration, and various measurement options.

- 2** Move the cursor to “Meas. Options” with the  or  button and press the  (Enter)/MENU button.



The <Meas. Options> screen is displayed.



# Display Type

|                     |               |
|---------------------|---------------|
| Meas. Options       | Page1/2       |
| Display Type        | : Absolute    |
| Color Space         | : E v / x / y |
| Meas. Time          | : AUTO        |
| Observer            | : 2°          |
| User cal.           | : UC00        |
| Select display type |               |

## [Operating Procedure]

- 1 On the <Meas. Options> screen, move the cursor to “Display Type” with the  or  button and press the  (Enter)/MENU button.

|                  |               |
|------------------|---------------|
| Display Type     | Page1/2       |
| Display Type     | : Absolute    |
|                  | : Difference  |
|                  | : Select Rank |
| Display absolute |               |

The <Display Type> screen is displayed.

- 2 Move the cursor to the item you wish to select with the  or  button.

|                    |               |
|--------------------|---------------|
| Display Type       | Page1/2       |
| Display Type       | : Absolute    |
|                    | : Difference  |
|                    | : Select Rank |
| Display difference |               |

Select the setting.

- 3 Press the  (Enter)/MENU button.

|                     |               |
|---------------------|---------------|
| Meas. Options       | Page1/2       |
| Display Type        | : Difference  |
| Color Space         | : E v / x / y |
| Meas. Time          | : AUTO        |
| Observer            | : 2°          |
| User cal.           | : UC00        |
| Select display type |               |

The selected content is confirmed and you return to the previous screen.

### Notes

If you press  without pressing , you return to the previous screen without changing the setting.

## Setting (● is the initial setting)

|   |                    |                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                 |
|---|--------------------|-----------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| ● | <b>Absolute</b>    | Displays the absolute value for the colorimetric value without using the target color.                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                          |
| ○ | <b>Difference</b>  | Displays the density difference for the target color.                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                           |
| ○ | <b>Select Rank</b> | <p>Displays a screen that ranks the chromaticity value within one of five fluorescent lamp classifications as defined by JIS Z 9221.</p> <ul style="list-style-type: none"> <li>• D (Daylight)</li> <li>• N (Natural)</li> <li>• W (White)</li> <li>• WW (Warm White)</li> <li>• L (Incandescent)</li> </ul> <p>“-----” (outside of ranks) is displayed when the chromaticity value is not within any of the ranks (chromaticity ranges).</p> <p>(Note, however, that the ranking result is not displayed when “CRI” or “Spectral” is selected for “Color Space”.</p> <p><b>Memo</b> You can use the CL-S10w data management software that comes with the instrument to modify the classification rank (chromaticity range) settings and the display names.</p> |

**Memo** For examples of the measurement condition screen in accordance with the items selected for the display type, see page E-33.

# Color Space

| Meas. Options      | Page1/2    |
|--------------------|------------|
| Display Type       | : Absolute |
| Color Space        | : Ev/x/y   |
| Meas. Time         | : AUTO     |
| Observer           | : 2°       |
| User cal.          | : UC00     |
| Select color space |            |

## [Operating Procedure]

- 1 On the <Meas. Options> screen, move the cursor to “Color Space” with the or button and press the (Enter)/MENU button.

| Color Space                   | Page1/2 |
|-------------------------------|---------|
| Ev/x/y                        |         |
| Ev/u/v                        |         |
| Ev/Tpc/Δuv                    |         |
| X/Y/Z                         |         |
| Ev/λ d/Pe                     |         |
| Show illuminance/chromaticity |         |

The <Color Space> screen is displayed.

- 2 Move the cursor to the item you wish to select with the or button.

| Color Space | Page1/2 |
|-------------|---------|
| Ev/x/y      |         |
| Ev/u/v      |         |
| Ev/Tpc/Δuv  |         |
| X/Y/Z       |         |
| Ev/λ d/Pe   |         |
| Show X/Y/Z  |         |

Select the setting.

- 3 Press the (Enter)/MENU button.

| Meas. Options      | Page1/2    |
|--------------------|------------|
| Display Type       | : Absolute |
| Color Space        | : X/Y/Z    |
| Meas. Time         | : AUTO     |
| Observer           | : 2°       |
| User cal.          | : UC00     |
| Select color space |            |

The selected content is confirmed and you return to the previous screen.

### Notes

If you press without pressing , you return to the previous screen without changing the setting.

Setting (● is the initial setting)

|   |            |                                                                                                       |
|---|------------|-------------------------------------------------------------------------------------------------------|
| ● | Ev/x/y     | Illuminance $E_v^{*1}$ , xy chromaticity                                                              |
| ○ | Ev/u/v'    | Illuminance $E_v^{*1}$ , u'v' chromaticity (CIE 1976 UCS Chromaticity Diagram)                        |
| ○ | Ev/Tcp/Δuv | Illuminance $E_v^{*1}$ , correlated color temperature Tcp, color difference Δuv from black body locus |
| ○ | X/Y/Z      | Tristimulus values X, Y, Z                                                                            |
| ○ | Ev/λd/Pe   | Illuminance $E_v^{*1}$ , dominant wavelength λ d, excitation purity $P_e^{*2}$                        |
| ○ | CRI        | Ra, R1-R15                                                                                            |
| ○ | Spectral   | Illuminance $E_v^{*1}$ spectral, peak wavelength                                                      |
| ○ | Custom     | Displays user-specified chromaticity values in measurement display items 1 through 4.                 |

\*1 Ev (Y of 2° field view) is displayed even when the observer is 10°.

\*2 The complementary wavelength value is displayed as a negative value when the “Display Type” setting is “Absolute” and the measured value is a non-spectral color.


In this case, the symbol remains λc.

When the “Display Type” setting is “Difference”, the difference between the measured value and the target is displayed, even if either the measured value and target or both of them are a complementary wavelength. In this case, the symbol is Δλ d when the target is a spectral color, regardless of its relationship with the measured value, and Δλ c when the target is a non-spectral color.

\* “---” is displayed when the calculated value is a combination that is rejected in the color space.


**Memo** For examples of the measurement condition screen in accordance with the items selected for the color space, see page E-33.

☐ Custom

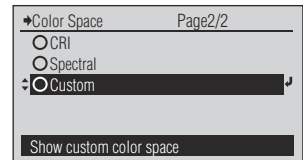


## [Operating Procedure]

- 1** On the <Color Space> screen, move the cursor to “Custom” with the or button and press the (Enter)/MENU button.



The <Custom> screen is displayed. Symbols in parentheses show what is displayed when the “Display Type” setting is “Difference”.


- 2** Move the cursor to “Color Space 1” with the or button and press the (Enter)/MENU button.




Color Space 1:  
Color space shown in item 1 of the measurement screen.  
{

Color Space 4:  
Color space shown in item 4 of the measurement screen.

- 3** Use the and buttons to move the cursor to “Color Space 2 through 4”.



- 4** Press the (Enter)/MENU button.




The selected content is confirmed and you return to the previous screen.

### Notes

If you press without pressing , you return to the previous screen without changing the setting.

- 5** Repeat steps 3 and 4 as required to configure settings for other items, and then press the button when you are done.




Returns to the <Color Space> screen.

# Meas. Time

| Meas. Options     | Page1/2       |
|-------------------|---------------|
| Display Type      | : Absolute    |
| Color Space       | : Ev/x/y      |
| Meas. Time        | : <b>AUTO</b> |
| Observer          | : 2°          |
| User cal.         | : UC00        |
| Select meas. time |               |


## [Operating Procedure]

- On the < Meas. Options> screen, move the cursor to “Meas. Time” with the or button and press the (Enter)/MENU button.




The <Meas. Time> screen is displayed.

- Move the cursor to the item you wish to select with the or button.



- Press the (Enter)/MENU button.



The selected content is confirmed and you return to the previous screen.

### Notes

If you press without pressing , you return to the previous screen without changing the setting.

## Setting (⊙ is the initial setting)

|                                  |             |                                                                                                                                                                                 |
|----------------------------------|-------------|---------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| <input type="radio"/>            | <b>FAST</b> | Mode that measures with a 0.5-second exposure time.                                                                                                                             |
| <input type="radio"/>            | <b>SLOW</b> | Mode that measures with a 2-second exposure time.                                                                                                                               |
| <input checked="" type="radio"/> | <b>AUTO</b> | High accuracy that automatically sets the exposure time (0.5 to 27 seconds) in accordance with the brightness of the light source being measured and then performs measurement. |

**Memo** The Accuracy and Repeatability values shown in the specifications (page E-72) are for when AUTO is selected. In the case of a short exposure time, Accuracy and Repeatability are lower at low illumination.

# Observer

| Meas. Options   | Page1/2    |
|-----------------|------------|
| Display Type    | : Absolute |
| Color Space     | : Ev/x/y   |
| Meas. Time      | : AUTO     |
| Observer        | : 2°       |
| User cal.       | : UC00     |
| Select observer |            |

## [Operating Procedure]

- 1 On the <Meas. Options> screen, move the cursor to “Observer” with the or button and press the (Enter)/MENU button.

| Observer        | Page1/1 |
|-----------------|---------|
| 2°              |         |
| 10°             |         |
| Select observer |         |

The <Observer> configuration screen is displayed.

- 2 Move the cursor to the item you wish to select with the or button.

| Observer        | Page1/1 |
|-----------------|---------|
| 2°              |         |
| 10°             |         |
| Select observer |         |

Select the setting.

- 3 Press the (Enter)/MENU button.

| Meas. Options   | Page1/2    |
|-----------------|------------|
| Display Type    | : Absolute |
| Color Space     | : Ev/x/y   |
| Meas. Time      | : AUTO     |
| Observer        | : 10°      |
| User cal.       | : UC00     |
| Select observer |            |

The selected content is confirmed and you return to the previous screen.


### Notes

If you press without pressing , you return to the previous screen without changing the setting.

**Setting** (● is the initial setting)


|  |     |                         |
|--|-----|-------------------------|
|  | 2°  | 2° observer (CIE 1931)  |
|  | 10° | 10° observer (CIE 1964) |

# Illum. Units




## [Operating Procedure]

- 1** On the <Meas. Options> screen, move the cursor to “Illum. Units” with the or button and press the (Enter)/MENU button.




The <Illum. Units> configuration screen is displayed.

- 2** Move the cursor to the item you wish to select with the or button.



Select the setting.

- 3** Press the (Enter)/MENU button.



The selected content is confirmed and you return to the previous screen.

### Notes

If you press without pressing , you return to the previous screen without changing the setting.

**Setting** (● is the initial setting)

|                                  |     |              |
|----------------------------------|-----|--------------|
| <input checked="" type="radio"/> | lx  | lux          |
| <input type="radio"/>            | fcd | foot-candela |

# User calibration

This instrument has 11 user calibration channels numbered UC00 to UC10.

UC00 is a channel for performing measurement in accordance with Konica Minolta calibration standards. Before your instrument is shipped from the factory, or during servicing or maintenance by Konica Minolta, the UC00 channel is preset with correction coefficients obtained during factory calibration. They correction coefficients cannot be changed by you.

Channels UC01 through UC10 can be configured with the settings below using the CL-S10w data management software that comes with your instrument as standard.

See the CL-S10w user documentation for information about actually using the software to configure settings.

- User calibration correction coefficients
- Correction coefficient name (ID)

The procedure below shows how to select a user calibration channel and how to change the items displayed in the list on the <User cal.> screen.

As necessary

Change settings.

## Selecting a User Calibration Channel

| Meas. Options         | Page1/2    |
|-----------------------|------------|
| Display Type          | : Absolute |
| Color Space           | : Ev/x/y   |
| Meas. Time            | : AUTO     |
| Observer              | : 2°       |
| ↓ User cal.           | : UC00     |
| Select user cal. data |            |

### [Operating Procedure]

- 1 On the < Meas. Options> screen, move the cursor to “User cal.” with the or button and press the (Enter)/MENU button.

| User cal.             | Page1/3 |
|-----------------------|---------|
| ○ UC00                |         |
| ○ UC01                |         |
| ○ UC02                |         |
| ○ UC03                |         |
| ○ UC04                |         |
| Select user cal. data |         |

The <User cal.> screen is displayed.

- 2 Move the cursor to the user calibration channel you want to select with the or button, and then press the (Enter)/MENU button.

| UC01                  | Page1/1     |
|-----------------------|-------------|
| ↓ Select              |             |
| List item             | : Date/Time |
| Select user cal. data |             |

The setting screen for the user calibration channel you selected appears.

- 3 Move the cursor to “Select” with the or button and press the (Enter)/MENU button.

| Meas. Options         | Page1/2    |
|-----------------------|------------|
| Display Type          | : Absolute |
| Color Space           | : Ev/x/y   |
| Meas. Time            | : AUTO     |
| Observer              | : 2°       |
| ↓ User cal.           | : UC01     |
| Select user cal. data |            |

The selected content is confirmed and you return to the previous screen.

#### Notes

If you press without pressing , you return to the previous screen without changing the setting.

# Changing the Items in the List on the <User cal.> Screen

| Meas. Options         | Page1/2    |
|-----------------------|------------|
| Display Type          | : Absolute |
| Color Space           | : Ev/x/y   |
| Meas. Time            | : AUTO     |
| Observer              | : 2°       |
| ✦ User cal.           | : UC00     |
| Select user cal. data |            |

## [Operating Procedure]

- On the < Meas. Options> screen, move the cursor to “User cal.” with the or button and press the (Enter)/MENU button.

| ✦ User cal.           | Page1/3 |
|-----------------------|---------|
| ✦ UC00                |         |
| ○ UC01                |         |
| ○ UC02                |         |
| ○ UC03                |         |
| ○ UC04                |         |
| Select user cal. data |         |

The <User cal.> screen is displayed.

- While the cursor is located at any user calibration channel, press the (Enter)/MENU button.

| ✦ UC00                | Page1/1     |
|-----------------------|-------------|
| ✦ Select              |             |
| List item             | : Date/Time |
| Select user cal. data |             |

The setting screen for the user calibration channel you selected appears.

- Move the cursor to “List item” with the or button and press the (Enter)/MENU button.

| ✦ List item                | Page1/1 |
|----------------------------|---------|
| ✦ Date/Time                |         |
| ○ Name                     |         |
| Show date/time registered. |         |

The <List item> screen is displayed.

- Use the and buttons to move the cursor to item you want to select, and then press the (Enter)/MENU button.

| ✦ UC00           | Page1/1 |
|------------------|---------|
| Select           |         |
| ✦ List item      | : Name  |
| Select list item |         |

This applies the settings for the selected item (regardless of which user calibration channel you originally selected) and returns to the previous screen.

### Notes

If you press without pressing , you return to the previous screen without changing the setting.

### Setting (⊙ is the initial setting)

|   |           |                                                                    |
|---|-----------|--------------------------------------------------------------------|
| ⊙ | Date/Time | Date and time a correction coefficient is registered               |
| ○ | Name      | Correction coefficient name (ID) (Name is specified with CL-S10w.) |



# Measurement

This chapter describes operating procedures for measurement functions. Set measurement conditions in advance as necessary before using each measurement function.

|                                                                    |      |
|--------------------------------------------------------------------|------|
| Measurement .....                                                  | E-32 |
| Measurement Screen .....                                           | E-33 |
| About Targets.....                                                 | E-34 |
| Registering a Target .....                                         | E-35 |
| Changing the Target .....                                          | E-36 |
| Deleting a Target.....                                             | E-37 |
| Changing the Items Displayed in the <Target data> Screen List..... | E-38 |
| Measured Data Operations .....                                     | E-39 |
| Registering Target Data.....                                       | E-40 |
| Deleting Measured Data.....                                        | E-41 |

# Measurement


Illuminance measurements are performed on the measurement screen.

A warm up period of at least 30 minutes is required under the following conditions to ensure good measurement accuracy.


- When the item being measured has low luminance (approximately 30 lx or less for Standard Illuminant A equivalent)
- When the ambient temperature of the measurement environment is outside the range of normal temperature

## [Operating Procedure]

- 1 Point the receptor window toward the illuminant to measure.

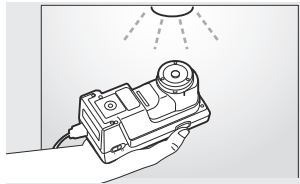

- 2 Press the measuring button.

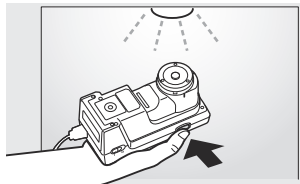

You will hear a beep.

- 3 The measurement is finished when you hear the beep again.

| 2°   AUTO   UC00   T01 |        |    |
|------------------------|--------|----|
| Ev                     | 240.2  | lx |
| x                      | 0.3642 |    |
| y                      | 0.3724 |    |
| Ready for measurement  |        |    |

The measurement value is displayed.

Next you can save measurement data.

- 4 Press the (Enter)/MENU button.

| Menu                          |   | Page1/2 |
|-------------------------------|---|---------|
| Save meas. data               |   |         |
| Zero cal.                     | + |         |
| Meas. Options                 | + |         |
| Meas. data                    | + |         |
| Target data                   | : | T01     |
| Save measurement data as M005 |   |         |

The <Menu> screen is displayed.

- 5 Press the (Enter)/MENU button with the cursor on "Save meas. data".

| 2°   AUTO   UC00   T01  |        |    |
|-------------------------|--------|----|
| Ev                      | 221.2  | lx |
| x                       | 0.3700 |    |
| y                       | 0.3779 |    |
| Measurement data saved. |        |    |























This saves the measurement data as measured data.

Up to a total of 100 measurement data items can be saved by the instrument in sequence from M001 to M100.

When measurement data is already saved up to M100, the <Overwrite> screen appears. If you decide to save your new data, the M001 data will be deleted, all data from M002 will be shifted up one position, and the new data will be saved as M100.

## Measurement Screen

The table below shows how measurement data is displayed in accordance with the display type and color space.

| Color Space | Display Type                                                                                                                                                                                             |                                                                                     |                                                                                                                                                                                                                                                                              | Color Space Explanation                                                                               |
|-------------|----------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|-------------------------------------------------------------------------------------|------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|-------------------------------------------------------------------------------------------------------|
|             | Absolute                                                                                                                                                                                                 | Select Rank                                                                         | Difference                                                                                                                                                                                                                                                                   |                                                                                                       |
| Ev/x/y      |                                                                                                                         |    |                                                                                                                                                                                             | Illuminance $E_v^{*1}$ , xy chromaticity                                                              |
| Ev/u'/v'    |                                                                                                                         |    |                                                                                                                                                                                             | Illuminance $E_v^{*1}$ , u'v' chromaticity (CIE 1976 UCS Chromaticity Diagram)                        |
| Ev/Tcp/Δuv  |                                                                                                                         |    |                                                                                                                                                                                             | Illuminance $E_v^{*1}$ , correlated color temperature Tcp, color difference Δuv from black body locus |
| X/Y/Z       |                                                                                                                         |    | <br> <p>Use the ▲ and ▼ buttons to switch between “Difference with Target” and “Percentage of Target”.</p> | Tristimulus values X, Y, Z                                                                            |
| Ev/λd/Pe    |                                                                                                                       |  |                                                                                                                                                                                           | Illuminance $E_v^{*1}$ , dominant wavelength λd, excitation purity $P_e^{*2}$                         |
| CRI         |  <p>Use the ▲ and ▼ buttons to switch between “R1 to R3”, “R4 to R6”, “R7 to R9”, “R10 to R12”, and “R13 to R15”.</p> |                                                                                     |  <p>Use the ▲ and ▼ buttons to switch between “ΔR1 to ΔR3”, “ΔR4 to ΔR6”, “ΔR7 to ΔR9”, “ΔR10 to ΔR12”, and “ΔR13 to ΔR15”.</p>                                                           | Ra, R1 to R15                                                                                         |
| Spectral    |                                                                                                                       |                                                                                     |                                                                                                                                                                                           | Spectral irradiance graph, peak wavelength                                                            |
| Custom      |                                                                                                                       |                                                                                     |                                                                                                                                                                                           | Displays user-specified chromaticity values in measurement display items 1 through 4.                 |

\*1  $E_v$  (Y of 2° field view) is displayed even when the observer is 10°.

\*2 The complementary wavelength value is displayed as a negative value when the “Display Type” setting is “Absolute” and the measured value is a non-spectral color.

In this case, the symbol remains λc.

When the “Display Type” setting is “Difference”, the difference between the measured value and the target is displayed, even if either the measured value and target or both of them are a complementary wavelength. In this case, the symbol is Δλ d when the target is a spectral color, regardless of its relationship with the measured value, and Δλ c when the target is a non-spectral color.

\* “---” is displayed when the calculated value is a combination that is rejected in the color space.

# About Targets

A target is a target color that is used during measurement to determine to what extent measured values deviate from a particular color.

A target is required when “Difference” is specified for the “Display Type” setting.

This instrument supports registration of up to a total of 20 targets, numbered T01 through T20.

To change the current target setting, perform the target selection procedure. Even if you change the target, the current user calibration correction coefficient does not change.

The target setting is common to each color space.

Target operations are performed on the <Target data> screen, which is accessed from the <Menu> screen.


Use the procedure below to display the <Target data> screen.

As necessary

Change settings.


## [Operating Procedure]

- 1** While the <measurement> screen is displayed, press the  (Enter)/MENU button.



The <Menu> screen is displayed.

- 2** Move the cursor to “Target data” with the  or  button and press the  (Enter)/MENU button.



The <Target data> screen is displayed.

## Registering a Target

The following are the different methods that can be used to register a target.

1. Registering measurement data
2. Registering selected measured data
3. Registering with the CL-S10w data management software that comes as standard with the instrument

See the CL-S10w user documentation for information about using the software to configure settings.

### [Operating Procedure]

**Memo** If you are planning to register measurement data as a target, you will need to perform the measurement before beginning the procedure below.

- 1 While the <Target data> screen is displayed, use the and buttons to move the cursor to the target number to which you want to register data (T01 through T20), and then press the (Enter)/MENU button.

|                 |     |     |     |
|-----------------|-----|-----|-----|
| •T01            | --- | --- | --- |
| Ev              | --- | Ix  |     |
| x               | --- |     |     |
| y               | --- |     |     |
| No target data. |     |     |     |

The screen for the target number you selected appears, showing any target data currently registered to that target number. If there is no data currently registered, “---” is displayed.

- 2 Press the (Enter)/MENU button.

|                             |             |
|-----------------------------|-------------|
| •T01                        | Page1/1     |
| ◀Select                     |             |
| Register                    | →           |
| List item                   | : Date/Time |
| Delete 1 Data               |             |
| Delete All                  |             |
| Use selected data as target |             |

The setting screen for the target number you selected appears.

- 3 Move the cursor to “Register” with the or button and press the (Enter)/MENU button.

|                          |                     |
|--------------------------|---------------------|
| •Register                | Page1/21            |
| ◀MEAS                    | 2011/12/24 11:03:51 |
| M001                     | 2011/12/24 10:54:21 |
| M002                     | 2011/12/24 10:05:07 |
| M003                     | 2011/12/24 10:55:07 |
| M004                     | 2011/12/24 10:55:07 |
| Select meas. data to use |                     |

The <Register> screen is displayed.

- 4 Use the and buttons to move the cursor to “MEAS” or to the number (M001 through M100) of the measured data you want to register, and then press the (Enter)/MENU button.

|                      |        |           |     |
|----------------------|--------|-----------|-----|
| •M001                | 2°     | AUTO/UC00 | T01 |
| Ev                   | 1570   | Ix        |     |
| x                    | 0.3753 |           |     |
| y                    | 0.3837 |           |     |
| Show meas. data M001 |        |           |     |

If you selected <MEAS>, the <MEAS> screen appears showing the new measurement data.

Or, the selected measured data screen is displayed and the measurement data appears.

- 5 Press the (Enter)/MENU button.

|                                               |
|-----------------------------------------------|
| •Confirm register                             |
| M001 will be registered as target number T01. |
| Continue?                                     |
| OK                                            |
| ◀Cancel                                       |
| Cancel registration                           |

The <Confirm register> or <Overwrite> screen appears.

- 6 Move the cursor to “OK” with the or button and press the (Enter)/MENU button.

|                        |                     |
|------------------------|---------------------|
| •Target data           | Page1/4             |
| ◀T01                   | 2011/12/24 10:54:21 |
| T02                    |                     |
| T03                    |                     |
| T04                    |                     |
| T05                    |                     |
| Target data registered |                     |

The data is registered to the selected target number and the <Target data> screen reappears.

# Changing the Target

You can select the target to be used for difference measurement by selecting one of the registered targets from T01 through T20.

The newly selected target is applied to the measurement values currently displayed on the measurement screen.

## [Operating Procedure]

**1** While the <Target data> screen is displayed, use the and buttons to move the cursor to the target number to which you want to select data (T01 through T20), and then press the (Enter)/MENU button.

|                      |        |      |  |
|----------------------|--------|------|--|
| •T02                 | 2°     | UC00 |  |
| Ev                   | 347.9  | Ix   |  |
| x                    | 0.3907 |      |  |
| y                    | 0.3886 |      |  |
| Show target data T02 |        |      |  |

The screen for the target number you selected appears, showing any target data currently registered to that target number. If there is no data currently registered, “---” is displayed.

**2** Press the (Enter)/MENU button.

|                             |             |
|-----------------------------|-------------|
| •T02                        | Page1/1     |
| Select                      |             |
| Register                    | •           |
| List item                   | : Date/Time |
| Delete 1 Data               |             |
| Delete All                  |             |
| Use selected data as target |             |

The screen for the target number you selected appears.

**3** Move the cursor to “Select” with the or button and press the (Enter)/MENU button.

|                                      |                     |
|--------------------------------------|---------------------|
| •Target data                         | Page1/4             |
| <input type="radio"/> T01            | 2011/12/24 15:32:31 |
| <input checked="" type="radio"/> T02 | 2011/12/24 15:32:31 |
| <input type="radio"/> T03            |                     |
| <input type="radio"/> T04            |                     |
| <input type="radio"/> T05            |                     |
| Selected target data changed         |                     |

The data is changed to the selected target number and the <Target data> screen reappears.

## Deleting a Target

You can use the procedure below to delete a registered target.

### [Operating Procedure]

- 1 While the <Target data> screen is displayed, use the  and  buttons to move the cursor to the target number to which you want to delete data (T01 through T20), and then press the  (Enter)/MENU button.

|                      |        |      |  |
|----------------------|--------|------|--|
| •T03                 | 2°     | UC00 |  |
| Ev                   | 1211   | Ix   |  |
| x                    | 0.3682 |      |  |
| y                    | 0.3785 |      |  |
| Show target data T03 |        |      |  |

The screen for the target number you selected appears, showing any target data currently registered to that target number. If there is no data currently registered, “---” is displayed.

- 2 Press the  (Enter)/MENU button.

|                             |             |  |  |
|-----------------------------|-------------|--|--|
| •T02                        | Page1/1     |  |  |
| ◀Select                     |             |  |  |
| Register                    | →           |  |  |
| List item                   | : Date/Time |  |  |
| Delete 1 Data               |             |  |  |
| Delete All                  |             |  |  |
| Use selected data as target |             |  |  |

The screen for the target number you selected appears.

- 3 Press the  (Enter)/MENU button, use the  and  buttons to move the cursor to “Delete 1 Data”, and then press the  (Enter)/MENU button.

|                                                     |  |  |  |
|-----------------------------------------------------|--|--|--|
| •Confirm deletion                                   |  |  |  |
| Selected target data T03 will be deleted. Continue? |  |  |  |
| OK                                                  |  |  |  |
| ◀Cancel                                             |  |  |  |
| Cancel deleting                                     |  |  |  |

The <Confirm deletion> screen is displayed.

- 4 Move the cursor to “OK” with the  or  button and press the  (Enter)/MENU button.

|                     |            |          |  |
|---------------------|------------|----------|--|
| •Target data        | Page1/4    |          |  |
| ○ T01               | 2011/12/24 | 10:54:21 |  |
| ○ T02               | 2011/12/24 | 10:55:07 |  |
| ◉ T03               |            |          |  |
| ○ T04               |            |          |  |
| ○ T05               |            |          |  |
| Target data deleted |            |          |  |

The target number data you selected is deleted and the <Target data> screen reappears.

#### **Memo**

If you selected “Delete All” in step 3, the data assigned to all target numbers is deleted.

# Changing the Items Displayed in the <Target data> Screen List

Use the procedure below to change the items displayed in the <Target data> screen list.

## [Operating Procedure]

- 1** While the <Target data> screen is displayed and the cursor is located at any target number, press the  (Enter)/MENU button.

|                      |        |      |  |
|----------------------|--------|------|--|
| •T02                 | 2°     | UC00 |  |
| Ev                   | 1211   | Ix   |  |
| x                    | 0.3682 |      |  |
| y                    | 0.3785 |      |  |
| Show target data T02 |        |      |  |

The screen for the target number that was selected appears, showing any target data currently registered to that target number. If there is no data currently registered, “---” is displayed.

- 2** Press the  (Enter)/MENU button.

|                             |             |
|-----------------------------|-------------|
| •T02                        | Page1/1     |
| ◀Select                     |             |
| Register                    | →           |
| List item                   | : Date/Time |
| Delete 1 Data               |             |
| Delete All                  |             |
| Use selected data as target |             |

The setting screen for the target number that was selected appears.

- 3** Move the cursor to “List item” with the  or  button and press the  (Enter)/MENU button.

|            |         |
|------------|---------|
| •List item | Page1/1 |
| ◀Date/Time |         |
| ○Name      |         |

The <List item> screen is displayed.

- 4** Use the  and  buttons to move the cursor to item you want to select, and then press the  (Enter)/MENU button.

|                  |         |
|------------------|---------|
| •T02             | Page1/1 |
| Select           |         |
| Register         | →       |
| ◀List item       | : Name  |
| Delete 1 Data    |         |
| Delete All       |         |
| Select list item |         |

This applies the settings for the selected item (regardless of which target number was originally selected) and returns to the previous screen.

### Notes

If you press  without pressing , you return to the previous screen without changing the setting.

**Setting** (◉ is the initial setting)

|   |                  |                                                                                                                                                  |
|---|------------------|--------------------------------------------------------------------------------------------------------------------------------------------------|
| ◉ | <b>Date/Time</b> | Date and time target data was measured                                                                                                           |
| ○ | <b>Name</b>      | Target data name (ID) (Target names cannot be edited. This is indicated on the display by square brackets [ ].)                                  |
|   |                  | <b>Memo</b> You can use the CL-S10w data management software that comes with the instrument to modify the target settings and the display names. |



# Measured Data Operations

Up to a total of 100 measurement data items can be saved by the instrument in sequence from M001 to M100. When measurement data is already saved up to M100, the <Overwrite> screen appears. If you decide to save your new data, the M001 data will be deleted, all data from M002 will be shifted up one position, and the new data will be saved as M100.

Measured data operations are performed on the <Meas. data> screen, which is accessed from the <Menu> screen. Use the procedure below to display the <Meas. data> screen.

## [Operating Procedure]

- 1 While the <measurement> screen is displayed, press the  (Enter)/MENU button.

| Menu                         |       | Page1/2 |
|------------------------------|-------|---------|
| Save meas. data              |       |         |
| Zero cal.                    | →     |         |
| Meas. Options                | →     |         |
| Meas. data                   | →     |         |
| Target data                  | : T02 |         |
| Show/delete saved meas. data |       |         |

The <MENU> screen is displayed.

- 2 Move the cursor to “Meas. data” with the  or  button and press the  (Enter)/MENU button.

| Meas. data               |                     | Page1/2 |
|--------------------------|---------------------|---------|
| M001                     | 2011/12/24 10:54:21 |         |
| M002                     | 2011/12/24 10:05:07 |         |
| M003                     | 2011/12/24 10:55:07 |         |
| M004                     | 2011/12/24 10:55:07 |         |
| M005                     | 2011/12/24 10:57:16 |         |
| Select meas. data to use |                     |         |

The <Meas. data> screen is displayed.

# Registering Target Data

In addition to the procedure shown on page E-35 of this manual, you also can use the procedure below to register target data.

## [Operating Procedure]

- While the <Meas. data> screen is displayed, use the and buttons to move the cursor to the measured data you want to select (M001 through M100), and then press the (Enter)/MENU button.

|                      |        |               |
|----------------------|--------|---------------|
| →M003                | 2°     | AUTO UC00 T01 |
| Ev                   | 1211   | Ix            |
| x                    | 0.3682 |               |
| y                    | 0.3785 |               |
| Show meas. data M003 |        |               |

The selected measured data screen is displayed and the measurement data appears. If there is no data currently stored, “---” is displayed.

- Press the (Enter)/MENU button.

|                               |         |
|-------------------------------|---------|
| →M003                         | Page1/1 |
| Register                      | →       |
| Delete 1 Data                 |         |
| Delete All                    |         |
| Set sel. meas. data as target |         |

The operation screen for the measured data number you selected appears.

- Move the cursor to “Register” with the or button and press the (Enter)/MENU button.

|                            |                     |
|----------------------------|---------------------|
| →Register                  | Page1/4             |
| ○T01                       | 2011/12/24 10:54:21 |
| ◉T02                       | 2011/12/24 10:55:07 |
| ○T03                       |                     |
| ○T04                       |                     |
| ○T05                       |                     |
| Select target data to use. |                     |

The <Register> screen is displayed.

- Use the and buttons to move the cursor to the target number to which you want to register data (T01 through T20), and then press the (Enter)/MENU button.

|                      |        |      |
|----------------------|--------|------|
| →T02                 | 2°     | UC00 |
| Ev                   | 1211   | Ix   |
| x                    | 0.3682 |      |
| y                    | 0.3785 |      |
| Show target data T02 |        |      |

The screen for the target number you selected appears, showing any target data currently registered to that target number. If there is no data currently registered, “---” is displayed.

- Press the (Enter)/MENU button.

|                                                           |
|-----------------------------------------------------------|
| →Overwrite                                                |
| Data already registered for target number T02. Overwrite? |
| OK                                                        |
| ←Cancel                                                   |
| Cancel overwriting                                        |

The <Confirm register> screen or the <Overwrite> screen is displayed.

- Move the cursor to “OK” with the or button and press the (Enter)/MENU button.

|                        |                     |
|------------------------|---------------------|
| →Meas. data            | Page1/20            |
| M001                   | 2011/12/24 10:54:21 |
| M002                   | 2011/12/24 10:05:07 |
| ◉M003                  | 2011/12/24 10:55:07 |
| M004                   | 2011/12/24 10:55:07 |
| M005                   | 2011/12/24 10:57:16 |
| Target data registered |                     |

The selected measured data is registered as a target and the <Meas. data> screen reappears.

## Deleting Measured Data

You can use the procedure below to delete measured data.

### [Operating Procedure]

- 1 While the <Meas. data> screen is displayed, use the and buttons to move the cursor to the measured data you want to delete (M001 through M100), and then press the (Enter)/MENU button.

|                      |        |      |      |     |
|----------------------|--------|------|------|-----|
| →M003                | 2°     | AUTO | UC00 | T01 |
| Ev                   | 1211   | Ix   |      |     |
| x                    | 0.3682 |      |      |     |
| y                    | 0.3785 |      |      |     |
| Show meas. data M003 |        |      |      |     |

The selected measured data screen is displayed and the measurement data appears. If there is no data currently stored, “---” is displayed.

- 2 Press the (Enter)/MENU button.

|                               |         |
|-------------------------------|---------|
| →M003                         | Page1/1 |
| Register                      | →       |
| Delete 1 Data                 |         |
| Delete All                    |         |
| Set sel. meas. data as target |         |

The operation screen for the measured data number you selected appears.

- 3 Move the cursor to “Delete 1 Data” with the or button and press the (Enter)/MENU button.

|                                                           |
|-----------------------------------------------------------|
| →Confirm deletion                                         |
| Selected measurement data M003 will be deleted. Continue? |
| OK                                                        |
| ←Cancel                                                   |
| Cancel deleting                                           |

The <Confirm deletion> screen is displayed.

- 4 Move the cursor to “OK” with the or button and press the (Enter)/MENU button.

|                           |                     |
|---------------------------|---------------------|
| →Meas. data               | Page1/20            |
| M001                      | 2011/12/24 10:54:21 |
| M002                      | 2011/12/24 10:05:07 |
| →M003                     | 2011/12/24 10:55:07 |
| M004                      | 2011/12/24 10:55:07 |
| M005                      | 2011/12/24 10:57:16 |
| Measurement data deleted. |                     |

The selected measured data is deleted and the <Meas. data> screen reappears. Deleting a data item causes the data items below it to shift upwards on the screen.

#### **Memo**

If you selected “Delete All” in step 3, all measured data is deleted.



# Other Functions

|                                                        |      |
|--------------------------------------------------------|------|
| Connecting to a PC .....                               | E-44 |
| CL-500A Settings .....                                 | E-46 |
| Buzzer Sound On/Off.....                               | E-47 |
| Invert Display.....                                    | E-48 |
| Configuring the Date and Time.....                     | E-49 |
| Configuring the Date Display Format.....               | E-50 |
| Auto Power Off Function.....                           | E-51 |
| Configuring the Zero Calibration Expiry .....          | E-52 |
| Turning Service Calibration Warning On or Off.....     | E-53 |
| Configuring the Display Language .....                 | E-54 |
| Initialize .....                                       | E-55 |
| Checking CL-500A Information.....                      | E-57 |
| Displaying Device Information.....                     | E-58 |
| Checking the Annual Service Recalibration Expiry ..... | E-59 |

## Connecting to a PC

The instrument is equipped with a USB connection terminal. Using the included USB cable, you can connect the instrument to a PC and transmit data.

**Notes**

- Do not connect a cable other than the designated cable to the USB connection terminal.
- When the instrument is connected to an external device and communicating with it, communications may be interrupted by being exposed to strong external static electricity or radio waves from the surrounding area. In these cases, turn the power OFF and then turn it ON again.

**Memo**

- When connected to a PC, the instrument automatically enters communication mode when the PC attempts to connect. “Communicating...” is displayed on the LCD screen, and the instrument’s control buttons and measuring button are disabled.
- When the command to enable the measuring button is used from the PC for the instrument, it is possible to measure by pressing the instrument’s measuring button.
- When connecting to the PC, we recommend using software that can connect to and use the instrument.
- The instrument’s USB communications port is USB 2.0 compliant.
- The instrument supports running on power from the USB cable.





**Notes**

- To connect the instrument to a PC, the dedicated USB driver must be installed. For the USB driver, use the driver included with the software that can connect to and use the instrument.
- Connect the USB connector plug firmly and with the correct orientation.
- Always connect and disconnect the USB cable by the connector’s plug. Do not pull it out by the cable itself or bend it with unreasonable force. Doing so may break the cable.
- Connect the instrument with a cable of a suitable length. If the cable lacks the suitable length, this may cause connection problems or cable breaks.
- Firmly push in the USB cable connector that matches the shape of the port (connection terminal) until it can go in no further.

## [Operating Procedure]

The USB cable can be connected and disconnected even when the instrument's power is ON, but here it is connected with the power turned OFF.

- 1** Turn OFF the instrument (Slide the Power switch to “O”).
- 2** Connect the USB cable's B connector to the instrument's USB connection terminal.
  - Firmly push it in until it can go no further and check that it is securely connected.
- 3** Connect the USB cable's A connector to the PC's USB port.
- 4** Turn ON the instrument (Slide the Power switch to “I”).
  - The PC recognizes the connection, and the USB driver is installed. Complete the installation. (Only when instrument is connected for the first time.)

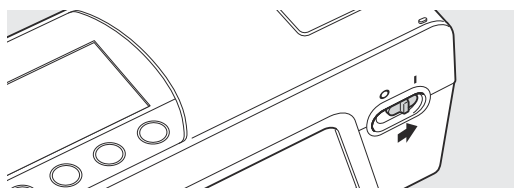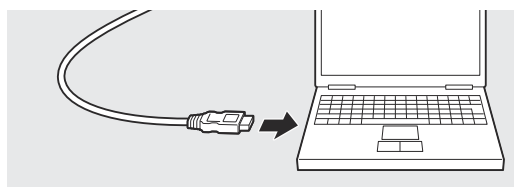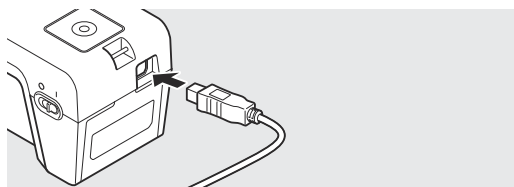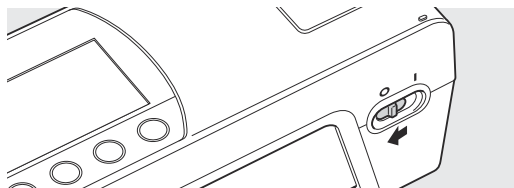

# CL-500A Settings

You set the display language for the instrument when first turning it on after purchase, but the other measuring instrument items are set with their initial settings, so the instrument can be used without configuring other settings.

Please change these settings as necessary.

Measuring instrument settings are configured on the <System> screen.


Move to the <System> screen with the procedure below.

As necessary

Change settings.


## [Operating Procedure]

- 1 While the measurement screen is displayed, press the  (Enter)/MENU button.



The <Menu> screen is displayed.

- 2 Move the cursor to “System” with the  or  button and press the  (Enter)/MENU button.



The <System> screen is displayed.

## Setting items

|                        |                                                        |
|------------------------|--------------------------------------------------------|
| <b>Buzzer</b>          | Changes the buzzer setting.                            |
| <b>Invert Display</b>  | Changes the orientation of the display.                |
| <b>Date/Time</b>       | Sets the display format for the current time and date. |
| <b>Auto Power Off</b>  | Changes the auto power off setting.                    |
| <b>Cal. Warning</b>    | Factory calibration expiry, etc.                       |
| <b>Language</b>        | Selects the display language.                          |
| <b>Initialize</b>      | Initializes the device's settings.                     |
| <b>Info(SerNo/Ver)</b> | Displays information about the device.                 |




# Buzzer Sound On/Off

You can switch the buzzer sound on and off.


## [Operating Procedure]

- 1 On the <System> screen, move the cursor to “Buzzer” with the or button and press the (Enter)/MENU button.




The <Buzzer> configuration screen is displayed.

- 2 Move the cursor to the item you wish to select with the or button.



Select the setting.

- 3 Press the (Enter)/MENU button.



If you turned on the buzzer, it will sound once.

Your setting is applied and the display returns to the previous screen.

### Notes

If you press without pressing , you return to the previous screen without changing the setting.

**Setting** (● is the initial setting)


|                                  |                                                                                                |
|----------------------------------|------------------------------------------------------------------------------------------------|
| <input checked="" type="radio"/> | On: The buzzer sounds when measurement starts and stops, and when a button is pressed.         |
| <input type="radio"/>            | Off: The buzzer does not sound when measurement starts and stops, or when a button is pressed. |

# Invert Display

You can flip the display on the LCD screen vertically.


## [Operating Procedure]

- 1** On the <System> screen, move the cursor to “Invert Display” with the  or  button and press the  (Enter)/MENU button.



The display on the LCD screen is flipped vertically.

- 2** Press the  button.



You return to the previous screen.

### Notes


If you press  without pressing  in step 1, you return to the previous screen without changing the setting.

## Configuring the Date and Time

The instrument contains an internal clock and records the measurement date and time when measuring. You can change the date and time.


### [Operating Procedure]

- 1 On the <System> screen, move the cursor to “Date/Time” with the  or  button and press the  (Enter)/MENU button.




The <Date/Time> screen is displayed.

- 2 Move the cursor to “Date/Time” with the  or  button and press the  (Enter)/MENU button.



The <Date/Time> configuration screen is displayed.

- 3 Set the year/month/day/hour/minute/second. Press the  button to increase the selected value or the  button to decrease it. Holding down either button will change the selected value at high speed. Press the  (Enter)/MENU button for each value to apply its setting.




This applies the changes you made to the setting and moves the cursor to the next value to the right.

#### Memo

Note that you cannot move the cursor to the left during the setting procedure.

- 4 While the cursor is located at the rightmost value (seconds), press the  (Enter)/MENU button.



All of your settings are applied and the display returns to the previous screen.

#### Notes


Pressing  without pressing  during this procedure will return to the previous screen without changing any of the settings.

# Configuring the Date Display Format

You can change the date display format.


## [Operating Procedure]

- 1** On the <System> screen, move the cursor to “Date/Time” with the  or  button and press the  (Enter)/MENU button.




The <Date/Time> screen is displayed.

- 2** Move the cursor to “Date Format” with the  or  button and press the  (Enter)/MENU button.




The <Date Format> screen is displayed.

- 3** Move the cursor to the item you wish to select with the  or  button.



Select the setting.

- 4** Press the  (Enter)/MENU button.



Your setting is applied and the display returns to the previous screen.

### Notes

If you press  without pressing , you return to the previous screen without changing the setting.

**Setting** (● is the initial setting)

|                                  |                   |                                           |
|----------------------------------|-------------------|-------------------------------------------|
| <input checked="" type="radio"/> | <b>yyyy/mm/dd</b> | Display the date in year/month/day order. |
| <input type="radio"/>            | <b>mm/dd/yyyy</b> | Display the date in month/day/year order. |
| <input type="radio"/>            | <b>dd/mm/yyyy</b> | Display the date in day/month/year order. |


# Auto Power Off Function

This instrument has an auto power off function. When running the instrument on its built-in lithium-ion battery without AC adapter or USB bus power, auto power off automatically turns power OFF if no control button operation is performed for more than 15 minutes.

You can enable or disable the auto power off function as required.


## [Operating Procedure]

- 1 On the <System> screen, move the cursor to “Auto Power Off” with the or button and press the (Enter)/MENU button.




The <Auto Power Off> screen is displayed.

- 2 Move the cursor to the item you wish to select with the or button.



Select the setting.

- 3 Press the (Enter)/MENU button.



Your setting is applied and the display returns to the previous screen.

### Notes

If you press without pressing , you return to the previous screen without changing the setting.

### Setting (● is the initial setting)

|                                  |                                                                                                                   |
|----------------------------------|-------------------------------------------------------------------------------------------------------------------|
| <input checked="" type="radio"/> | On: Power turns off automatically if no button operation on the instrument is performed for more than 15 minutes. |
| <input type="radio"/>            | Off: Auto power off not performed.                                                                                |


# Configuring the Zero Calibration Expiry

The instrument displays the calibration prompt screen when a fixed amount of time elapses from the last white calibration. The initial setting for this calibration expiry is set to 12 hours when shipped from the factory. You can change this zero calibration expiry.

**Memo** Frequent short zero calibration is recommended for better accuracy when measuring low illuminance.


## [Operating Procedure]

- 1 On the <System> screen, move the cursor to “Cal. Warning” with the  or  button and press the  (Enter)/MENU button.




The <Cal. Warning> screen is displayed.

- 2 Move the cursor to “Cal. Warning” with the  or  button and press the  (Enter)/MENU button.




The <Cal. Warning> screen is displayed.

- 3 Move the cursor to the item you wish to select with the  or  button.



Select the setting.

- 4 Press the  (Enter)/MENU button.



Your setting is applied and the display returns to the previous screen.

### Notes

If you press  without pressing , you return to the previous screen without changing the setting.

### Setting (⊙ is the initial setting)

|                                  |           |                                                                                                                                                                                               |
|----------------------------------|-----------|-----------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| <input type="radio"/>            | 3h        |                                                                                                                                                                                               |
| <input type="radio"/>            | 6h        |                                                                                                                                                                                               |
| <input checked="" type="radio"/> | 12h       |                                                                                                                                                                                               |
| <input type="radio"/>            | 24h       |                                                                                                                                                                                               |
| <input type="radio"/>            | No Expiry | The calibration prompt screen is not displayed.<br><b>Memo</b> Even when “No Expiry” is selected, the calibration prompt screen may appear if there is a large change in ambient temperature. |


# Turning Service Calibration Warning On or Off

When the service calibration warning feature of this instrument is enabled, a message is displayed when the instrument is turned on to suggest periodic calibration about one year after shipment from the factor or after the last calibration service or maintenance was performed on the instrument.

You can use the procedure below to disable display of the service calibration warning message.


## [Operating Procedure]

- 1 On the <System> screen, move the cursor to “Cal. Warning” with the  or  button and press the  (Enter)/MENU button.




The <Cal. Warning> screen is displayed.

- 2 Move the cursor to “Svc. Cal. Warn.” with the  or  button and press the  (Enter)/MENU button.




The <Svc. Cal. Warn.> screen is displayed.

- 3 Move the cursor to the item you wish to select with the  or  button.



Select the setting.

- 4 Press the  (Enter)/MENU button.



Your setting is applied and the display returns to the previous screen.

### Notes

If you press  without pressing , you return to the previous screen without changing the setting.

Setting (⊙ is the initial setting)


|                                  |                                                                    |
|----------------------------------|--------------------------------------------------------------------|
| <input checked="" type="radio"/> | On: Enables display of the periodic calibration warning message.   |
| <input type="radio"/>            | Off: Disables display of the periodic calibration warning message. |

# Configuring the Display Language

You can change the display language from the language set when the power was first turned on after purchase.


## [Operating Procedure]

- 1** On the <System> screen, move the cursor to “Language” with the or button and press the (Enter)/MENU button.




The <Language> screen is displayed.

- 2** Move the cursor to the item you wish to select with the or button.




Select the setting.

- 3** Move the cursor to the item you wish to select with the or button.



The <Confirm Change> screen is displayed.

- 4** Move the cursor to “OK” with the or button, then press the (Enter)/MENU button.



Your setting is applied and the display returns to the previous screen.

**Notes**  
If you press without pressing , you return to the previous screen without changing the setting.

**Setting** (● is the initial setting)

|                                  |          |
|----------------------------------|----------|
| <input checked="" type="radio"/> | English  |
| <input type="radio"/>            | Japanese |
| <input type="radio"/>            | Chinese  |




# Initialize

Returns the settings for the instrument back to their initial state.

- Notes
- Do not initialize the instrument except when necessary.
  - When the instrument is initialized, the zero calibration execution records and target color data are deleted.


## [Operating Procedure]

- 1
- On the <System> screen, move the cursor to “Initialize” with the  or  button and press the  (Enter)/MENU button.



The <Initialize> screen is displayed. The cursor is initially on “Cancel”.

- 2
- Move the cursor to “OK” with the  or  button and press the  (Enter)/MENU button.




The instrument is initialized.

Memo

The instrument does not restart. The display language for the LCD screen changes to English, the initial setting.

- 3
- Press the  button.



You return to the previous screen.

## Initial settings

| Item          |                |                          | Initial setting               |
|---------------|----------------|--------------------------|-------------------------------|
| Meas. Options | Display Type   |                          | Absolute                      |
|               | Color Space    |                          | Ev/x/y                        |
|               | Meas. Time     |                          | AUTO                          |
|               | Observer       |                          | 2°                            |
|               | Illum. Units   |                          | lx                            |
|               | User cal.      | User calibration channel | (UC01 to UC10) not registered |
| Zero cal.     |                |                          | UC00 (factory calibration)    |
| Target data   |                |                          | Not completed                 |
|               | Target data    |                          | Not registered                |
| Meas. data    |                |                          | T00                           |
| Select Rank   |                |                          | Not completed                 |
|               |                |                          | D (Daylight)                  |
|               |                |                          | N (Natural)                   |
|               |                |                          | W (White)                     |
|               |                |                          | WW (Warm White)               |
| System        |                |                          | L                             |
|               | Buzzer         |                          | On                            |
|               | Invert Display |                          | Normal                        |
|               | Date/Time      | Date Format              | yyyy/mm/dd                    |
|               | Auto Power Off |                          | On                            |
|               | Cal. Warning   | 0-cal. warning           | 12h                           |
|               |                | Svc. Cal. Warn.          | On                            |
|               | Language       |                          | English                       |


\* Instrument settings may be initialized by causes other than the initialize operation (such as complete discharge of the built-in battery).

# Checking CL-500A Information

You can check information about the instrument.  
Check measuring instrument information on the <System> screen. Move to the <System> screen with the procedure below.


## [Operating Procedure]

- 1** While the measurement screen, press the  (Enter)/MENU button.



The <Menu> screen is displayed.

- 2** Move the cursor to “System” with the  or  button and press the  (Enter)/MENU button.




The <System> screen is displayed.

# Displaying Device Information

The instrument’s model name, serial number, and version are displayed.


## [Operating Procedure]

- 1** On the <System> screen, move the cursor to “Info(SerNo/Ver)” with the  or  button and press the  (Enter)/MENU button.



The <Info(SerNo/Ver)> screen is displayed.

- 2** When finished checking the information, press the  button.



You return to the previous screen.


# Checking the Annual Service Recalibration Expiry

After approximately one year elapses after the instrument is shipped from the factory or after KONICA MINOLTA SENSING calibration service (or maintenance), a message will be displayed when the power is turned on that recommends annual service recalibration.

You can check the time limit until the annual service recalibration recommendation message is next displayed here.

## [Operating Procedure]

- 1** On the <System> screen, move the cursor to “Cal. Warning” with the  or  button and press the  (Enter)/MENU button.




The <Cal. Warning> screen is displayed.

- 2** Move the cursor to “Svc. Cal. Expir” with the  or  button and press the  (Enter)/MENU button.



The <Svc. Cal. Expir> configuration screen is displayed, and the time limit when the next factory calibration is required is shown.

- 3** Press the  button.



You return to the previous screen.



# Troubleshooting

|                                           |      |
|-------------------------------------------|------|
| Error Messages .....                      | E-62 |
| Checking for Malfunction .....            | E-64 |
| Special Startup Procedures .....          | E-65 |
| Initialization .....                      | E-65 |
| Starting Up from the Language Screen..... | E-65 |

## Error Messages

The messages below may be displayed when using the instrument. When one of these messages is displayed, please take the action indicated below. When you perform the action but the instrument does not return to normal, or when the power does not turn on even when the internal battery is charged, contact a KONICA MINOLTA SENSING-authorized service facility.

**Notes** • The messages below may be displayed on the LCD screen. Refer to the separate materials for the communication error check codes.

| No. | Error Message                                                                   | Problem/possible cause                                                                                                                                                                                                               | Action                                                                                                                                         |
|-----|---------------------------------------------------------------------------------|--------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|------------------------------------------------------------------------------------------------------------------------------------------------|
| 1   | Perform zero calibration.<br>Press [MEAS] button to start zero calibration.     | Measurement performed without zero calibration.                                                                                                                                                                                      | Perform zero calibration.                                                                                                                      |
| 2   | Error. Calibrate again.                                                         | Some abnormality occurred during calibration.                                                                                                                                                                                        | Perform zero calibration again. If this message continues to appear, immediately contact a KONICA MINOLTA SENSING-authorized service facility. |
| 3   | Zero calibration recommended.<br>Press [MEAS] button to start zero calibration. | The zero calibration warning time limit has expired. Or there was a large change in ambient temperature since the last zero calibration was performed.                                                                               | Perform zero calibration.                                                                                                                      |
| 4   | No measurement data.                                                            | There is no data registered to the selected measured data number.                                                                                                                                                                    | Select a measured data number that has data and try again.                                                                                     |
| 5   | No target data.                                                                 | There is no data registered to the selected target number.                                                                                                                                                                           | Select a target number that has data and try again.                                                                                            |
| 6   | No user cal. data.                                                              | There is no data registered to the selected user calibration channel.                                                                                                                                                                | Select a user calibration channel that has data and try again.                                                                                 |
| 7   | Input value outside range.<br>Enter again.                                      | A non-existent date was input.                                                                                                                                                                                                       | Re-input a valid date.                                                                                                                         |
| 8   | Over measurement range.                                                         | The illuminance exceeds the level that can be measured by the CL-500A.                                                                                                                                                               | Increase the distance between the CL-500 and the light source being measured, or use an ND filter to reduce the intensity of the light.        |
| 9   | Chroma at < 5 lx out of spec.                                                   | The illuminance obtained by the measurement is less than 5 lx, so chromaticity calculation performance is low.                                                                                                                       | Decrease the distance between the CL-500 and the light source being measured, or increase the intensity of the light.                          |
| 10  | More error at set meas. time.                                                   | Any one of the following can cause failure to satisfy Accuracy specifications.<br>• Less than 50 lx obtained by measurement when measurement time is FAST<br>• Less than 10 lx obtained by measurement when measurement time is SLOW | Change the measurement time setting to AUTO and measure again.                                                                                 |
| 11  | Over dom. wl. calc. range.                                                      | The dominant wavelength could not be calculated.                                                                                                                                                                                     | The dominant wavelength cannot be calculated with the light source being used. This does not indicate malfunction.                             |
| 12  | Over Tcp calc. range.                                                           | The correlated color temperature could not be calculated.                                                                                                                                                                            | The correlated color temperature cannot be calculated with the light source being used. This does not indicate malfunction.                    |



| No. | Error Message                                            | Problem/possible cause                                                                                          | Action                                                                                                                                                                                                                                    |
|-----|----------------------------------------------------------|-----------------------------------------------------------------------------------------------------------------|-------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| 13  | Over CRI calc. range.                                    | The CRI could not be calculated.                                                                                | The CRI cannot be calculated with the light source being used. This does not indicate malfunction.                                                                                                                                        |
| 14  | No custom color space is set.                            | The settings of none of the items from Color Space 1 through 4 are configured. ("None" selected for all items.) | Configure the settings of one of the items from Color Space 1 through Color Space 4. Or change to another Color Space.                                                                                                                    |
| 15  | No valid rank list is set.                               | The chromaticity range settings required to perform ranking are not configured.                                 | Use the CL-S10w data management software that comes with the instrument as standard to configure the rank list.                                                                                                                           |
| 16  | Battery voltage is low.<br>Recharge battery.             | Battery voltage is low and there is enough for only a small number of measurements.                             | Use the AC adapter or USB power bus to charge the battery.<br>The instrument may not start up immediately after the AC adapter is connected. In this case, allow the battery to charge for a few minutes and then turn on the instrument. |
| 17  | The battery is degrading.<br>Contact Service Center.     | An abnormality was detected in the battery.                                                                     | Immediately stop using the instrument and contact a KONICA MINOLTA SENSING-authorized service facility.                                                                                                                                   |
| 18  | Circuit malfunction.<br>Contact Service Center.          | An abnormality was detected in the measurement circuit, etc.                                                    | Immediately stop using the instrument and contact a KONICA MINOLTA SENSING-authorized service facility.                                                                                                                                   |
| 19  | Clock malfunction.<br>Charge battery. Set clock.         | An abnormality was detected in the clock data.<br>• Battery voltage may be too low.                             | Use the AC adapter or USB power bus to charge the battery, and then set the correct time and date.                                                                                                                                        |
| 20  | Time for service calibration.<br>Contact Service Center. | It is time to perform periodic calibration.                                                                     | Contact a KONICA MINOLTA SENSING-authorized service facility and request periodic calibration.                                                                                                                                            |

## Checking for Malfunction

In the event that something goes wrong with the instrument, carry out the measures below. If the instrument does not return to normal, try turning the power off. If this does not work, contact the nearest KONICA MINOLTA SENSING-authorized service facility.


| Condition                                                | Cause                                                                                                             | Action                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                          |
|----------------------------------------------------------|-------------------------------------------------------------------------------------------------------------------|-----------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| The LCD is blank.                                        | Is the battery low?                                                                                               | Charge the instrument using the AC adapter or USB bus power.<br>If the instrument does not work even after the battery has been charged, it is possible that overcurrent may have occurred and burned out the internal fuse. Immediately stop using the instrument and contact a KONICA MINOLTA SENSING-authorized service facility.                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                            |
|                                                          | If recharging the battery does not solve the problem, it could mean there is some problem with the CPU.           | While instrument power is turned on, hold down the  button and the  button for at least four seconds. This will reset the CPU and restart the CL-500A.<br><b>Notes</b><br>Performing the reset operation will result in the following.<br><ul style="list-style-type: none"> <li>• Data measured immediately prior to the reset will be lost.</li> <li>• Target data (including names) saved the last time power was turned on, changed settings (including display language), and zero calibration records may be deleted.</li> </ul> If your display language setting is deleted, use the procedure under “Starting Up from the Language Screen” on page E-65 to display the <Language> screen and select the display language you want. |
|                                                          | If resetting the CPU does not solve the problem, it could mean that over current has blown the instrument’s fuse. | Immediately stop using the instrument and contact a KONICA MINOLTA SENSING-authorized service facility.                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                         |
| Measurement results are abnormal.                        | Did you perform zero calibration correctly?                                                                       | Use the cap and correctly perform zero calibration.                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                             |
| The instrument cannot be controlled from a PC.           | Is the USB cable connected correctly?                                                                             | Connect the USB connection terminal on the instrument correctly to the PC’s USB port using the USB cable supplied as a standard accessory.                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                      |
|                                                          | Are you using the USB cable supplied as a standard accessory?                                                     |                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                 |
|                                                          | Is the CL-500A being correctly recognized by the PC as a USB device?                                              | Refer to the installation guide that comes with the CL-S10w (Ver.1.1 or greater) software and reinstall the USB device driver.                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                  |
| The battery is low even though it has just been charged. | The internal lithium-ion battery can be charged around 500 times.                                                 | If the battery is low even though it has just been fully charged, the battery must be replaced. Contact the nearest KONICA MINOLTA SENSING-authorized service facility.                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                         |

# Special Startup Procedures

## Initialization

While holding down the  button and  button, slide the power switch to the “I” side. This will start up the instrument from the <Initialize> screen.


For information about the <Initialize> screen, refer to page E-55.

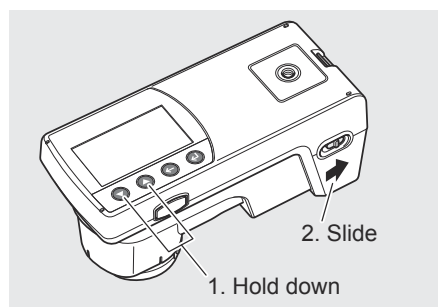

## Starting Up from the Language Screen

While holding down the  (Enter)/MENU button, slide the power switch to the “I” side. This will start up the instrument from the <Language> screen.

For information about the <Language> screen, refer to page E-54.

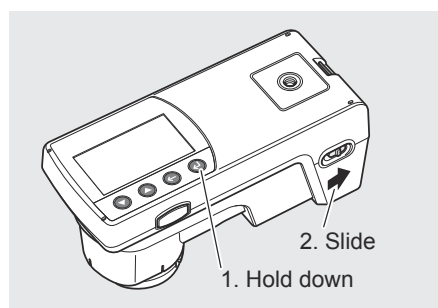



# Appendix

|                                             |      |
|---------------------------------------------|------|
| Luminance Measurement Capabilities .....    | E-68 |
| Relative Spectral Response .....            | E-68 |
| Cosine Correction Characteristics .....     | E-68 |
| LvTΔuv .....                                | E-69 |
| Dominant wavelength/Excitation purity ..... | E-70 |
| External Dimensions .....                   | E-71 |
| Specifications .....                        | E-72 |

6

Before Using the  
Instrument

Preparation for  
Measurement

Measurement

Other Functions


Troubleshooting

Appendix

# Luminance Measurement Capabilities

## Relative Spectral Response


The spectral response of an ideal illuminance meter would match  $V(\lambda)$ , the spectral luminance efficiency function for photopic vision. JIS (Japan Industrial Standards) has established a rating system that classifies illuminance meters according to how closely they match this function. The CL-500A CHROMA METER conforms to the “general class AA” classification.

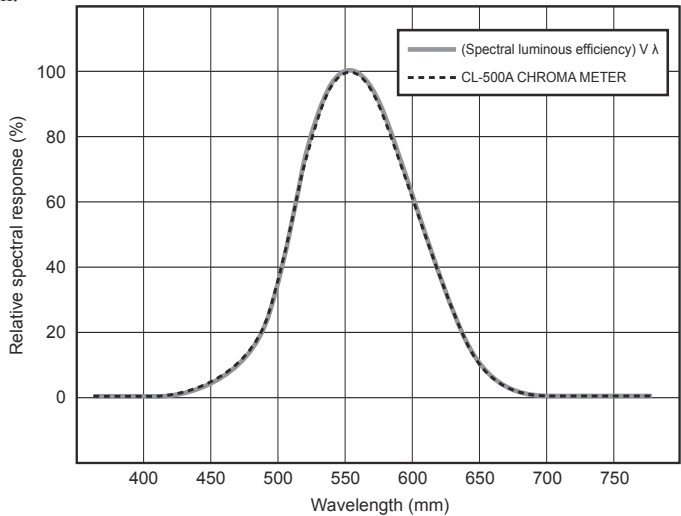

## Cosine Correction Characteristics

Because the brightness at the measurement plane is proportional to the cosine of the angle of incidence, the response of the receptor must also be proportional to this cosine.

The graph below shows the cosine correction characteristics of the CL-500A CHROMA METER. This instrument conforms to the “general class AA” classification.

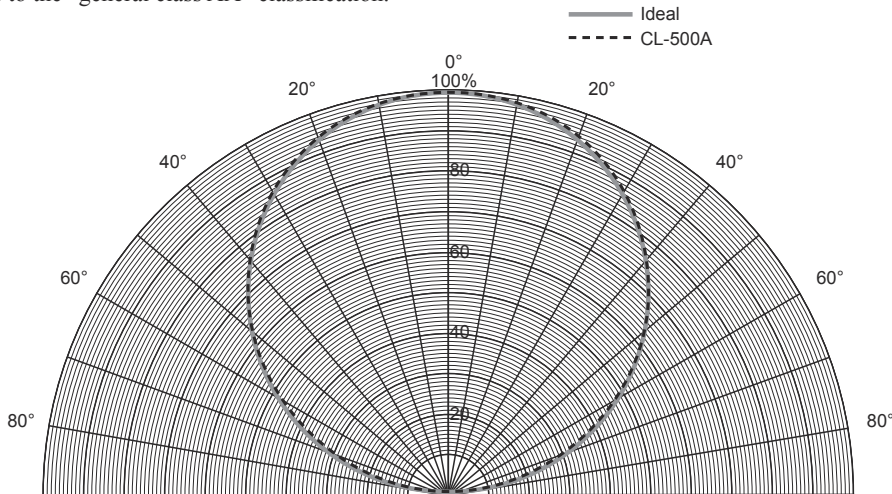

# LvTΔuv

Following factors can be acquired as measurement value with  $L_vT\Delta uv$  as color space of this instrument.

$L_v$  : Luminance

$T$  :Correlated color temperature

$\Delta uv$  :Color difference from blackbody locus

While  $L_{vs}$  stands for luminance,  $T$  and  $\Delta uv$  for color in  $L_vT\Delta uv$ .

## <Relation between correlated color temperature $T$ and color difference from blackbody locus $\Delta uv$ >


Color temperature refers to the temperature of black body (perfect radiator) which has equal chromaticity coordinates to certain light. However, color temperature only represents colors on blackbody locus.

Correlated color temperature, slightly wider interpretation of color temperature, is very useful to eliminate such problem. Here, correlated color temperature covers those which are slightly outside the range of that of blackbody locus.

If a certain color positions on isothermperature line, the intersection point of isothermperature line and blackbody locus is indicated as correlated color temperature for the color. Isothermperature line means line on chromaticity coordinates which is a set of colors visually close to color temperature on blackbody locus.

However, since all colors on a color-matching temperature line are represented with equal correlated color temperature, it is not possible to describe color only with correlated color temperature. To solve that,  $\Delta uv$ , deviation of correlated color temperature  $T$  from blackbody locus, is to apply for that purpose.

If  $\Delta uv$  exists above blackbody locus, it is represented with “+”, and below, with “-”.

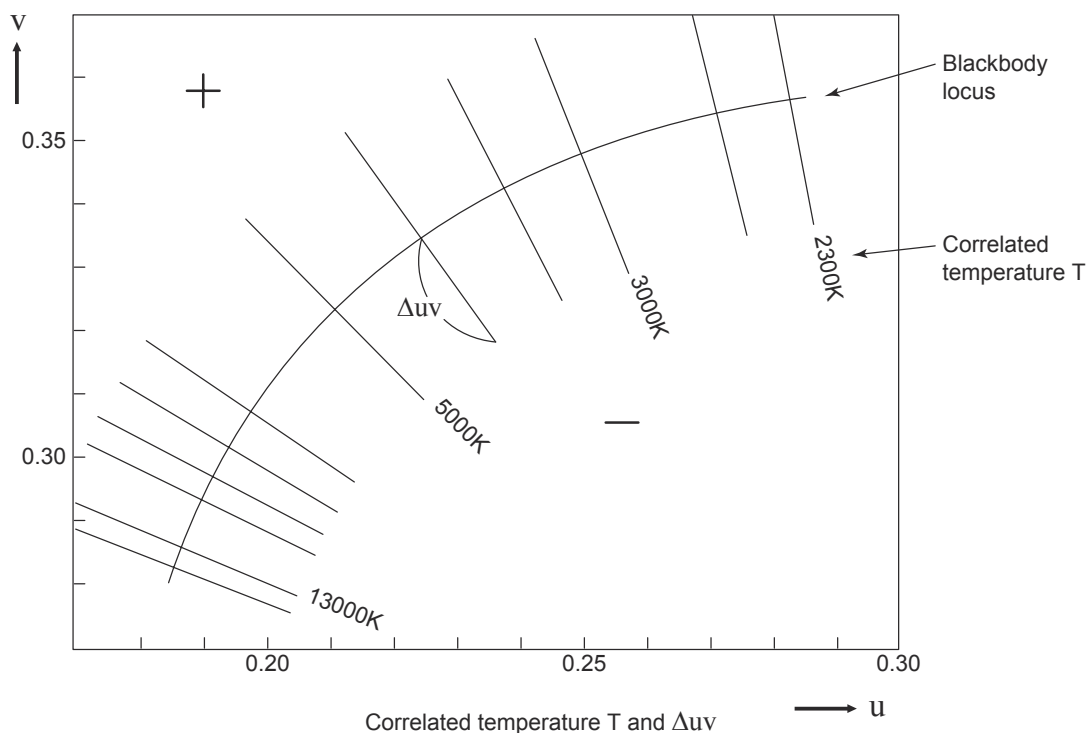

## Dominant wavelength/Excitation purity

In the  $x, y$  chromaticity diagram shown below, the curve  $VS_cSR$  is the spectrum locus, and point  $N$  is the white point.

Colors located in the region enclosed by the spectrum locus and the straight lines  $VN$  and  $NR$  are referred to as spectral colors; colors located in the triangle  $NVR$  with the white point  $N$  at the apex and the pure purple line  $VR$  as the base are referred to as nonspectral colors.

### <Dominant wavelength and excitation purity (spectral colors)>

When the chromaticity point obtained by the measurement is  $C$ , the wavelength corresponding to the intersection point  $S$  of the extension of  $NC$  with the spectrum locus (curve  $VS_cSR$ ) is referred to as the dominant wavelength and indicated by the symbol  $\lambda_d$ .

The ratio of the lengths of the straight lines  $NC$  and  $NS$  is referred to as the excitation purity of color excitation  $C$  and indicated by the symbol  $p_c$ .

### <Complementary wavelength (non-spectral colors)>

When the chromaticity point obtained by measurement is  $C'$ , the extension of  $NC'$  toward  $C'$  does not intersect with the spectrum locus but only the pure-purple lines. In this case the wavelength corresponding to the intersection point  $S_c$  of the extension of  $NC'$  toward  $N$  with the spectrum locus is referred to as the complementary wavelength and indicated by the symbol  $\lambda_c$ .

When the intersection point of the extension of the line  $NC'$  with the line  $VR$  (pure-purple locus) is designated by  $S'$ , the ratio of the lengths of  $NC'$  to  $NS'$  is referred to as excitation purity and indicated by the symbol  $p'_v$ .


The following equations are formulated, if each point is designated as the following coordinates:  $(x_n, y_n)$ : chromaticity coordinate of point  $N$ ;  $(x_c, y_c)$ : chromaticity coordinate of point  $C$ ;  $(x_s, y_s)$ : chromaticity coordinate of point  $S$ ;  $(x'_c, y'_c)$ : chromaticity coordinate of point  $C'$ , and  $(x_p, y_p)$ : chromaticity coordinate of point:

Excitation purity (spectral colors)

$$p_c = \frac{x_c - x_n}{x_s - x_n} = \frac{y_c - y_n}{y_s - y_n}$$

Excitation purity (non-spectral colors)

$$p'_c = \frac{x'_c - x_n}{x_p - x_n} = \frac{y'_c - y_n}{y_p - y_n}$$

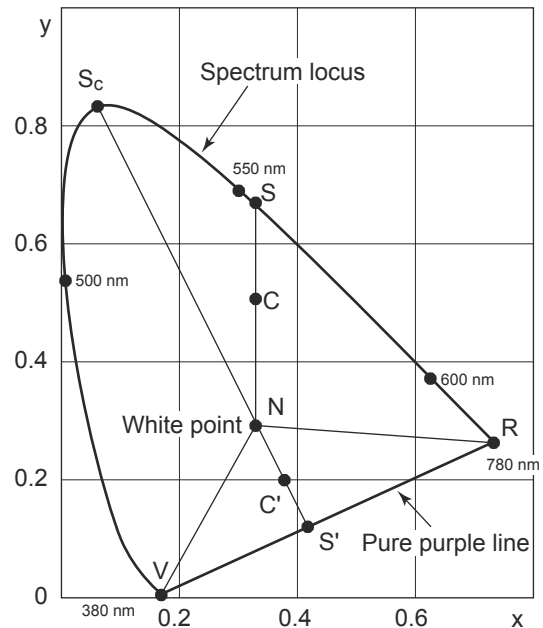


Dominant wavelength on chromaticity diagram



# External Dimensions

(Unit: mm)

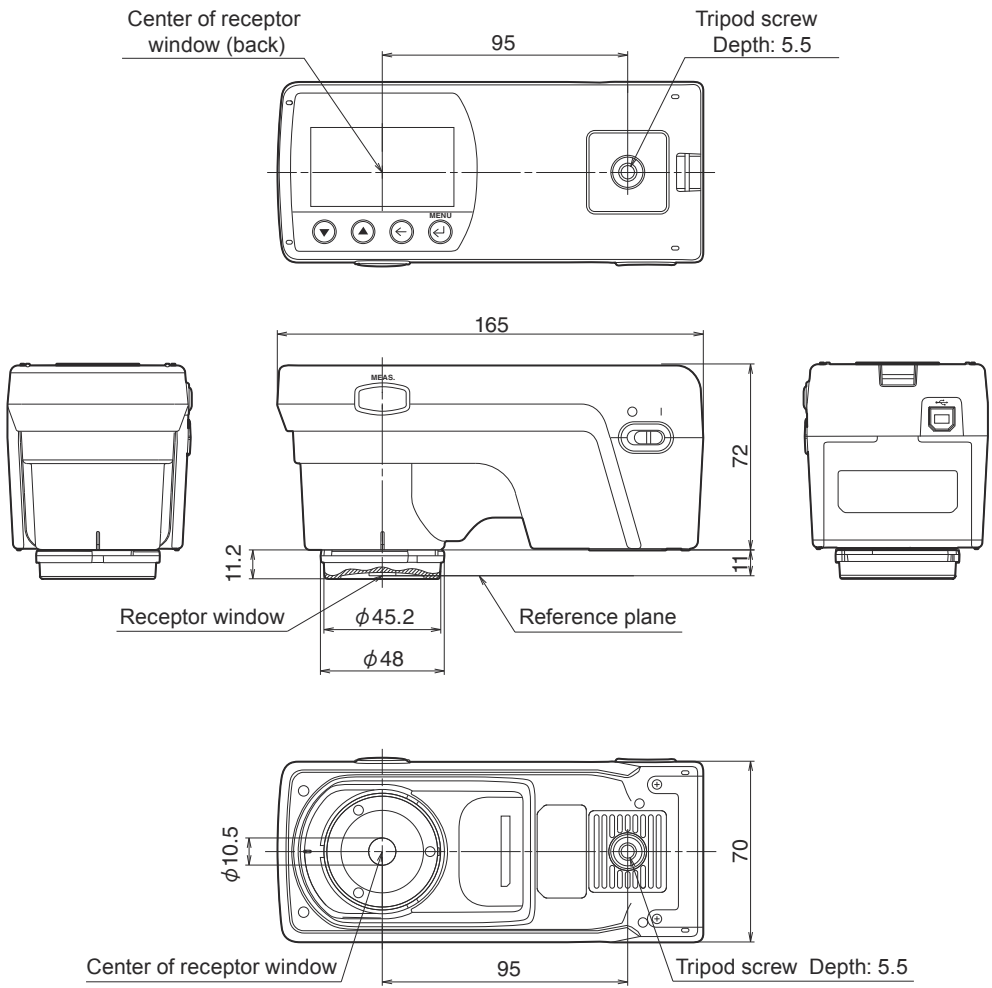

# Specifications

|                                                                             |                                                                                                                                                                                                                                                                                                                                                                               |                                                     |
|-----------------------------------------------------------------------------|-------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|-----------------------------------------------------|
| Model name                                                                  | Illuminance Spectrophotometer CL-500A                                                                                                                                                                                                                                                                                                                                         |                                                     |
| Illuminance meter class                                                     | Conforms to JIS C 1609-1: 2006 for General Class AA Illuminance Meters <sup>*1</sup><br>Conforms to DIN 5032 Part 7 Class B                                                                                                                                                                                                                                                   |                                                     |
| Spectral wavelength range                                                   | 360 to 780 nm                                                                                                                                                                                                                                                                                                                                                                 |                                                     |
| Output wavelength pitch                                                     | 1 nm                                                                                                                                                                                                                                                                                                                                                                          |                                                     |
| Spectral bandwidth                                                          | Approximately 10 nm (half bandwidth)                                                                                                                                                                                                                                                                                                                                          |                                                     |
| Wavelength precision                                                        | ±0.3 nm (Median wavelengths of 435.8 nm, 546.1 nm, and 585.3 nm <sup>*2</sup> as specified in JIS Z 8724) <sup>*3</sup>                                                                                                                                                                                                                                                       |                                                     |
| Measuring range                                                             | 0.1 to 100,000 lx (Chromaticity display requires at least 5 lx.)                                                                                                                                                                                                                                                                                                              |                                                     |
| Accuracy <sup>*4</sup> <sup>*5</sup><br>(Standard Illuminant A)             | Ev: ±2% ±1digit of displayed value<br>xy: ±0.0015 (500 to 100,000 lx)                                                                                                                                                                                                                                                                                                         | xy: ±0.002 (5 to 10 lx)                             |
| Repeatability (2σ) <sup>*4</sup><br>(Standard Illuminant A)                 | Ev: 0.5% + 1digit<br>xy: 0.0005 (500 to 100,000 lx)<br>xy: 0.002 (30 to 100 lx)                                                                                                                                                                                                                                                                                               | xy: 0.001 (100 to 500 lx)<br>xy: 0.004 (5 to 30 lx) |
| Visible-region relative spectral response characteristics (f <sub>1</sub> ) | 1.5% or less                                                                                                                                                                                                                                                                                                                                                                  |                                                     |
| Cosine response (f <sub>2</sub> )                                           | Ev: 3% or less                                                                                                                                                                                                                                                                                                                                                                |                                                     |
| Temperature drift (f <sub>T</sub> )                                         | Ev: ±3% of displayed value<br>Xy: ±0.003                                                                                                                                                                                                                                                                                                                                      |                                                     |
| Humidity drift (f <sub>H</sub> )                                            | Ev: ±3% of displayed value<br>Xy: ±0.003                                                                                                                                                                                                                                                                                                                                      |                                                     |
| Measurement Time                                                            | Super Fast Mode: Approximately 0.2 seconds (When connected to PC only)<br>FAST Mode: Approximately 0.5 seconds<br>SLOW Mode: Approximately 2.5 seconds<br>Automatic exposure time setting (high accuracy mode): Approximately 0.5 to 27 seconds                                                                                                                               |                                                     |
| Display Modes                                                               | XYZ; X <sub>10</sub> Y <sub>10</sub> Z <sub>10</sub> ; Ev xy; Ev u'v'; dominant wavelength; excitation purity; Ev; Correlated color temperature; Δuv; General color-rendering index (Ra); Special color-rendering indexes (Ri (i=1-15)); spectral graph; peak wavelength; Δ (XYZ); Δ (X <sub>10</sub> Y <sub>10</sub> Z <sub>10</sub> ); Δ (Ev xy); Δ (Ev u'v'); rank display |                                                     |
| Other Functions                                                             | Data memory: 100 items; user calibration (when connected to computer); continuous measurement (when connected to computer); auto power off                                                                                                                                                                                                                                    |                                                     |
| Display Languages                                                           | Japanese, English, Chinese                                                                                                                                                                                                                                                                                                                                                    |                                                     |
| Interface                                                                   | USB2.0                                                                                                                                                                                                                                                                                                                                                                        |                                                     |
| Power                                                                       | Built-in lithium-ion battery *Possible operation time:6 hours operation (between full charges, for a new product); AC adapter; USB power bus                                                                                                                                                                                                                                  |                                                     |
| Operation temperature and humidity ranges                                   | -10 to 40°C, relative humidity of 85% or less (at 35°C) with no condensation                                                                                                                                                                                                                                                                                                  |                                                     |
| Storage temperature and humidity ranges                                     | -10 to 45°C, relative humidity of 85% or less (at 35°C) with no condensation                                                                                                                                                                                                                                                                                                  |                                                     |
| Dimensions                                                                  | 70 (W) x 165 (D) x 83 (H) mm                                                                                                                                                                                                                                                                                                                                                  |                                                     |
| Weight                                                                      | 350 g                                                                                                                                                                                                                                                                                                                                                                         |                                                     |

\*1 "Section 7.6.3 Response Time" conforms when measurement speed mode is FAST.

\*2 585.3 nm evaluation performed using substitute wavelength of 587.6 nm.

\*3 Based on Konica Minolta test standards (2°C or less temperature change after zero calibration).

\*4 Automatic exposure time setting (high accuracy) mode

\*5 Linear for Ev (illuminance)



KONICA MINOLTA